


RV Investigator

CTD Processing Report

Voyage ID:	in2021_v03
Voyage title:	Integrated Marine Observing System: Monitoring of the East Australian Current Property Transports at 27°S
Depart:	Hobart, 0800 Thursday, 8 May 2021
Return:	Brisbane, 0800 Thursday, 3 June 2021

Document History

Date	Version	Author	Comments
24/05/2021	1.0	Ella Pietraroia	Initial version
23/07/2021	2.0	Ella Pietraroia	Date change

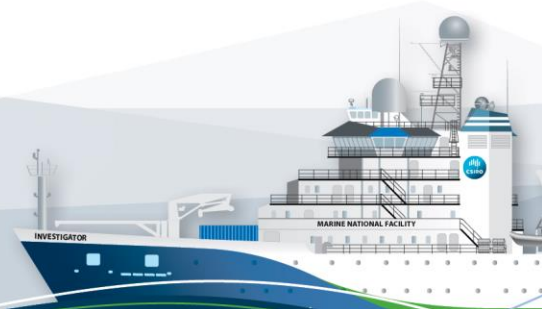

Contents

1	Summary	3
2	Voyage Details	3
2.1	Title	3
2.2	Principal Investigators	3
2.3	Voyage Objectives	3
2.4	Area of operation	4
3	Processing Notes.....	6
3.1	Background Information.....	6
3.2	Pressure and temperature calibration	7
3.3	Conductivity Calibration	8
3.4	Dissolved Oxygen Sensor Calibration	10
3.4.1	SBE calibration procedure	10
3.4.2	Results	10
3.5	Other sensors	12
3.6	Bad data detection	12
3.7	Heave Filtering.....	13
3.8	Averaging.....	13
4	References	13
	Appendix I: Conductivity Calibration Residual Plots	15
	Appendix II: Dissolved Oxygen Calibration Residual Plots.....	16

1 Summary

These notes relate to the production of quality controlled, calibrated CTD data from RV Investigator voyage in2021_v03, from 08 May 2021 – 04 Jun 2021.

Data for 36 deployments were acquired using the Sea-Bird SBE911 CTD 24, fitted with 19 twelve litre bottles on the rosette sampler. Sea-Bird-supplied calibration factors were used to compute the pressures and preliminary conductivity values. CSIRO -supplied calibrations were applied to the temperature data. The data were subjected to automated QC to remove spikes and out-of-range values.

The final conductivity calibration was based on a single deployment grouping. The final calibration from the primary sensor had a standard deviation (SD) of 0.0019084 PSU, when rounded this is outside our target of 'better than 0.002 PSU', so the cut-off was adjusted to 0.003 PSU. The standard product of 1 decibar binned averaged were produced using data from the primary sensors.

Cast 10 was ended prematurely so CapPro could not process cast properly. To overcome this, in MATLAB, the end of cast 9 was attached to the end of cast 10. This data will not appear in the raw files from SeaSave and should not affect processing, as CapPro will remove out of water data before processing but needs this data to find the end of the cast.

During cast 12 the CTD landed on the bottom of the ocean floor, no damage was found, and all subsequent casts performed as expected.

Prior to cast 31, due to some discrepancies between the primary and secondary sensors, the Seagoing Instrumentation Team swapped the secondary pump. This resolved the particular issue.

Bottle seven had intermittent problems firing reliably. Initially the release magnet was swapped and all further casts had a backup fired with bottle 7, however it was later found that the root cause was corrosion under the epoxy. As a precaution, the whole trigger mechanism was swapped.

The dissolved oxygen data calibration fit had a SD of 0.84461 μ M. The agreement between the CTD and bottle data was good.

PAR, Transmissometer, CDOM, Altimeter and Ecotriplet were also installed on the auxiliary A/D channels of the CTD.

2 Voyage Details

2.1 Title

Integrated Marine Observing System: Monitoring of the East Australian Current Property Transports at 27°S

2.2 Principal Investigators


Bernadette Sloyan, Amandine Schaeffer, Iain Suthers, Kylie Pitt

2.3 Voyage Objectives

The scientific objectives for in2021_v03 were outlined in the Voyage Plan.

For further details, refer to the Voyage Plan and/or summary which can be viewed on the Marine National Facility web site.

2.4 Area of operation

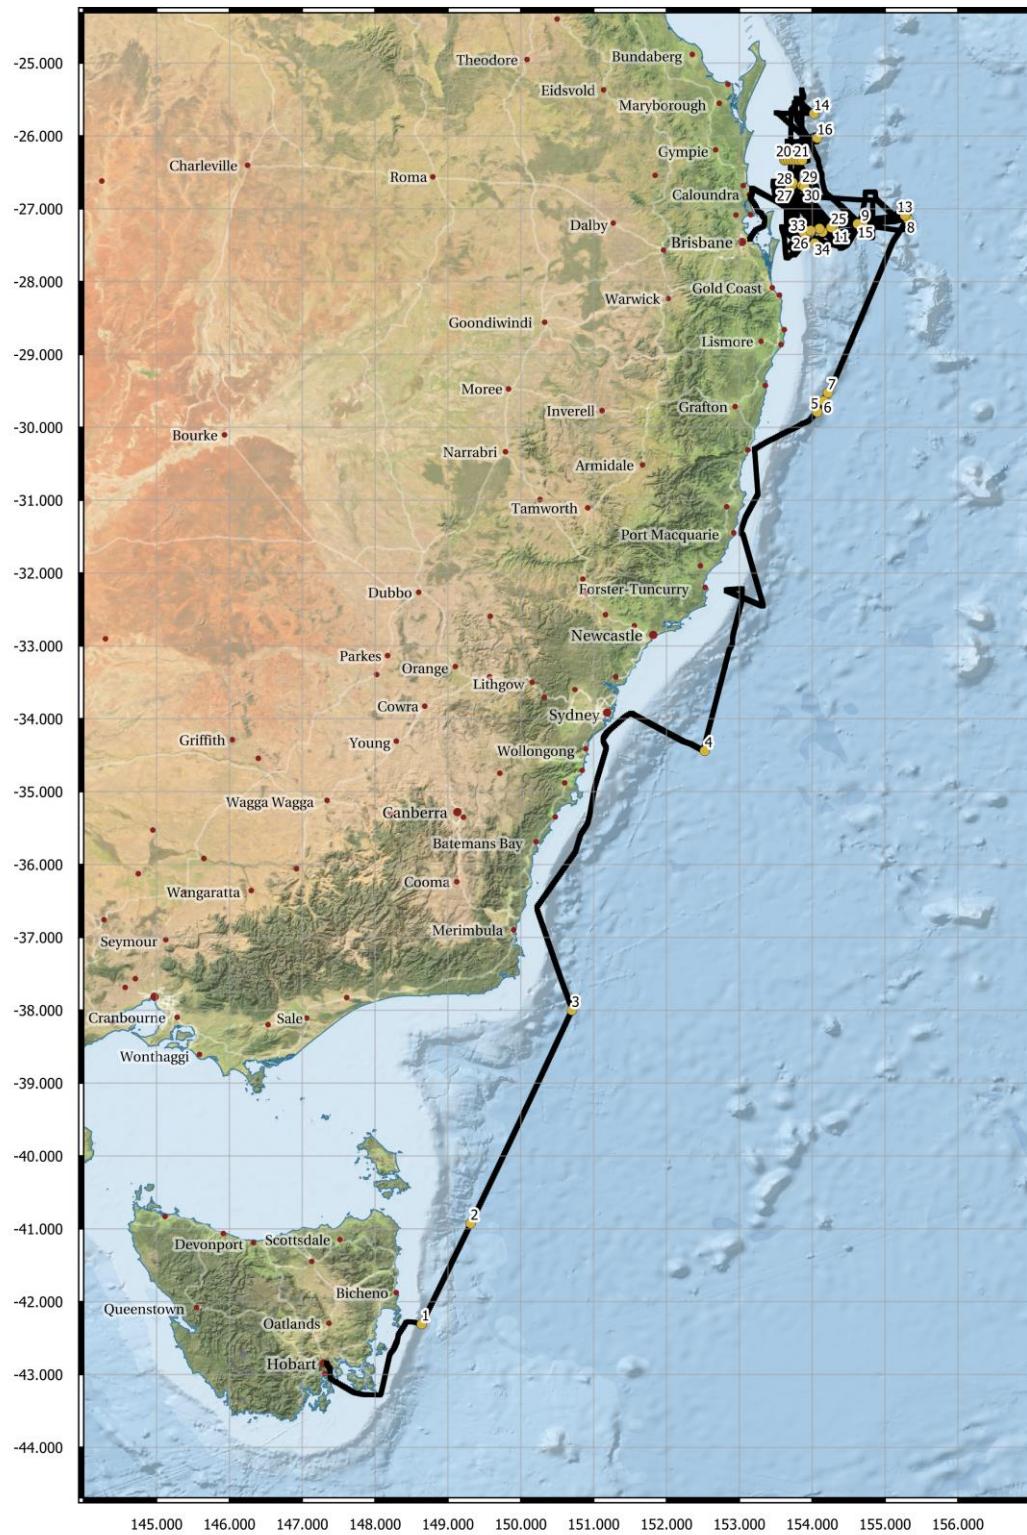

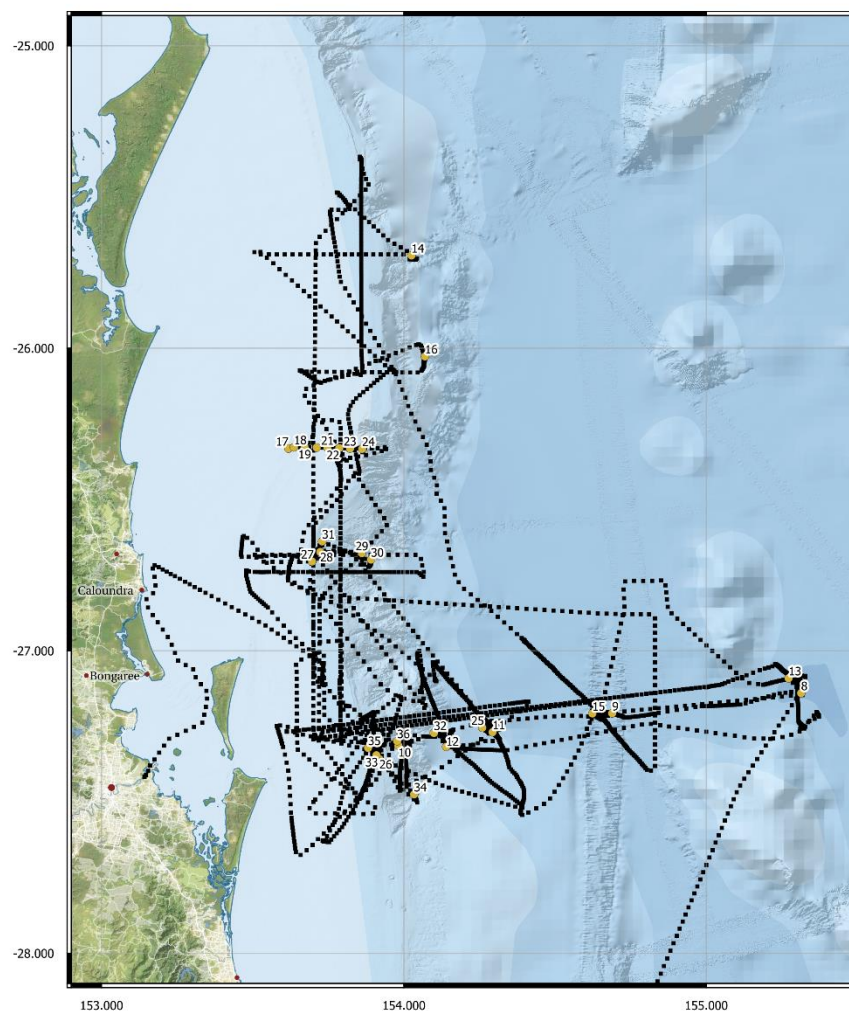


Figure 1 Area of operation for in2021_v03

3 Processing Notes

3.1 Background Information

The data for this voyage were acquired with the CSIRO CTD unit 24, a Sea-Bird SBE911 with dual conductivity and temperature sensors.

The CTD was additionally fitted with SBE43 dissolved oxygen sensors , transmissometer, Wetlabs FLBBRTD, altimeter and Wetlabs FLCDRD. These sensors are described in

PAR	Biospherical QCP2300HP	70111	A3	20-Oct-2020	Biospherical
Transmissometer	Wetlabs C-Star	CST-2009DR	A4	28-Oct-2020	Wet Labs
CDOM	Wetlabs FLCDRD	4367	A5	18-May-2020	Wet Labs
Wetlabs ECO - Chlorophyll	FLBB	5169	A6	18-May-2020	Wet Labs
Wetlabs ECO - Scattering	FLBB	5169	A7	19-Nov-2020	Wet Labs

Table 1 below.

Description	Sensor	Serial No.	A/D	Calibration Date	Calibration Source
Pressure	Digiquartz 410K-134	1332	P	2-Jul-2020	CSIRO Cal Lab
Primary Temperature	Sea-Bird SBE3T	6180	T0	23-Jan-2021	CSIRO Cal Lab
Secondary Temperature	Sea-Bird SBE3T	6285	T1	25-Sep-2020	CSIRO Cal Lab
Primary Conductivity	Sea-Bird SBE4C	4773	C0	21-Sep-2021	CSIRO Cal Lab
Secondary Conductivity	Sea-Bird SBE4C	4774	C1	21-Sep-2020	CSIRO Cal Lab
Primary Dissolved Oxygen	SBE43	3155	A0	14-Oct-2020	CSIRO Cal Lab
Secondary Dissolved Oxygen	SBE43	1794	A1	21-Nov-2020	Sea-Brid
Altimeter	Tritech PA500	228403	A2	28-May-2020	Tritech
PAR	Biospherical QCP2300HP	70111	A3	20-Oct-2020	Biospherical
Transmissometer	Wetlabs C-Star	CST-2009DR	A4	28-Oct-2020	Wet Labs
CDOM	Wetlabs FLCDRD	4367	A5	18-May-2020	Wet Labs
Wetlabs ECO - Chlorophyll	FLBB	5169	A6	18-May-2020	Wet Labs
Wetlabs ECO - Scattering	FLBB	5169	A7	19-Nov-2020	Wet Labs

Table 1 CTD Sensor configuration on in2021_v03

Water samples were collected using a Sea-Bird SBE32, 36-bottle rosette sampler. Sampling was from 19 twelve litre bottles which were fitted to the frame.

There were 36 deployments and of these, deployments none were on-deck TSG calibration runs.

The raw CTD data were collected in SBE SeaSave version 7.26.7.110, converted to scientific units using SBE Data Processing version 7.26.7.129 and written to NetCDF format files with CNV_to_Scan for processing using the Matlab-base, CapPro package version 2.11.

The CapPro software was used to apply automated QC and preliminary processing to the data. This included spike removal, identification of water entry and exit times, conductivity sensor lag corrections, conductivity cell thermal inertia corrections, and the determination of the pressure offsets. It also loaded

the hydrology data and computed the matching CTD sample burst data. The automatically determined pressure offsets and in-water points were inspected.

The bottle sample data were used to compute final conductivity and dissolved oxygen calibrations. These were applied to the data, after which files of binned 1 decibar averaged data were produced.

3.2 Pressure and temperature calibration

The pressure offsets are plotted in Figure 2 below. The blue circles refer to initial out-of-water values and the red circles the final out-of-water values. The value for deployment 10 is missing because the acquisition software was stopped too early. To ensure the processing software was able to run, entered out of water on-deck scan indexes manually by using Seabird processing software to plot cast, and copied reference pressure from cast 9 to cast 10. Processing worked well from there. Modified values saved in `ctd_processing\in2021_v03\in2021_v03_010_surf_values.mat`.

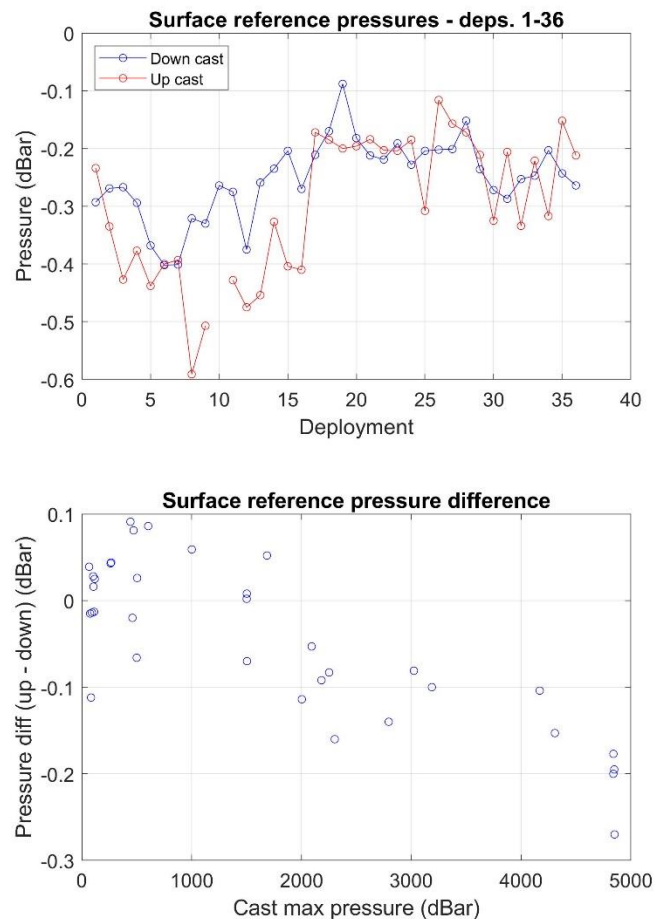


Figure 2 CTD pressure offsets

The difference between the primary and secondary temperature sensors at the bottle sampling depths is plotted below. Most deployments plot within $\pm 0.001^{\circ}\text{C}$ of zero – outliers result from sampling in regions of high vertical temperature gradient as supported by the similarity between the temperature and conductivity difference shown in Figure 3. This indicates neither sensor has drifted significantly from its calibration.

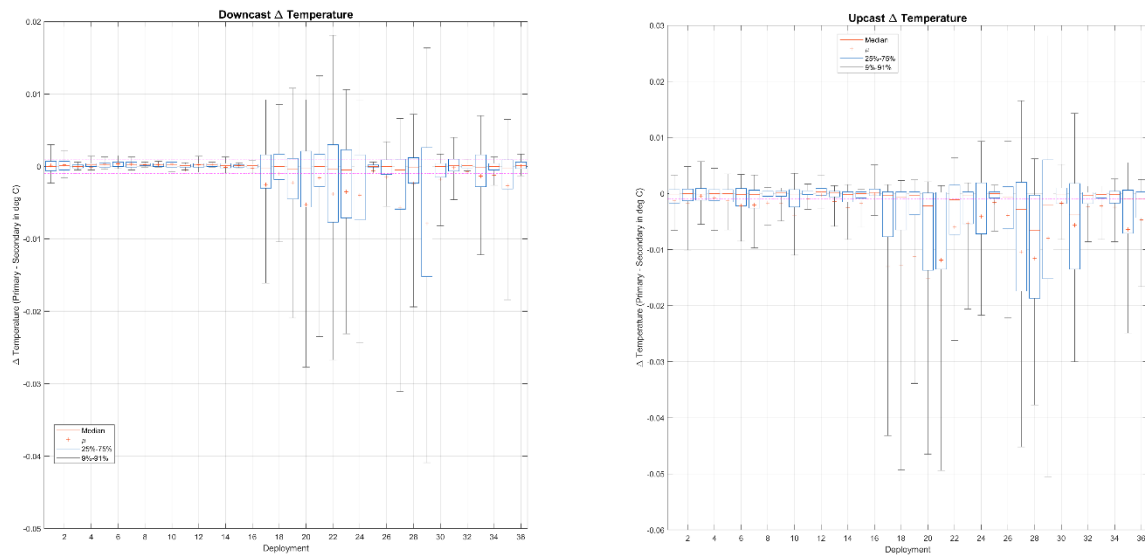


Figure 3 Difference between primary and secondary temperature sensors

3.3 Conductivity Calibration

Discrepancies and possible sampling problems between bottle and CTD salinities for the primary conductivity sensor would show in Figure 4; the plot of calibrated (CTD - Bottle) salinity below. The calibration was based upon the sample data (primary/secondary) for 218/217 of the total of 350 samples taken during deployments which are above our target of 70%, at a cut-off of 0.004.

The outliers marked in Figure 4 below with magenta dots are excluded from the calibration, the outliers marked with blue dots are used in the calibration but are weighted based on their distance from the mean. Any outliers marked with red crosses or dots are also excluded from the calibration.

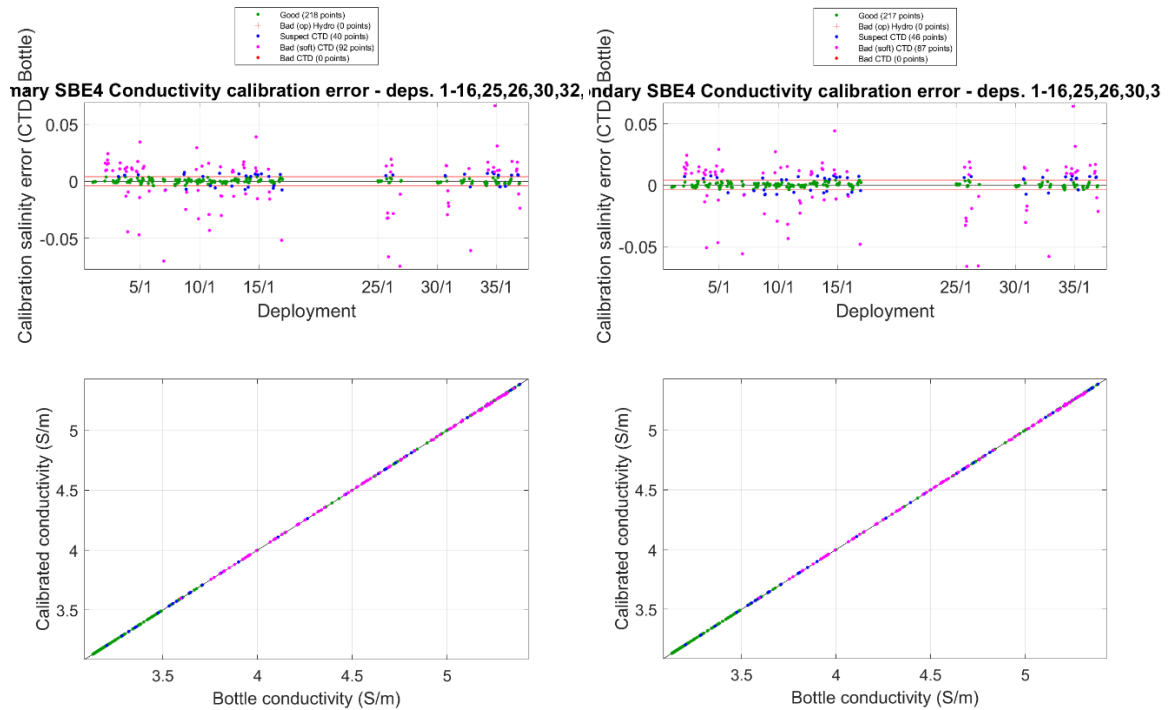


Figure 4 CTD - bottle salinity plot

The box plot of calibrated downcast conductivities (primary - secondary) at the bottle sampling depths for all deployments in Figure 5 shows that the calibrated conductivity cell responses corresponded very well.

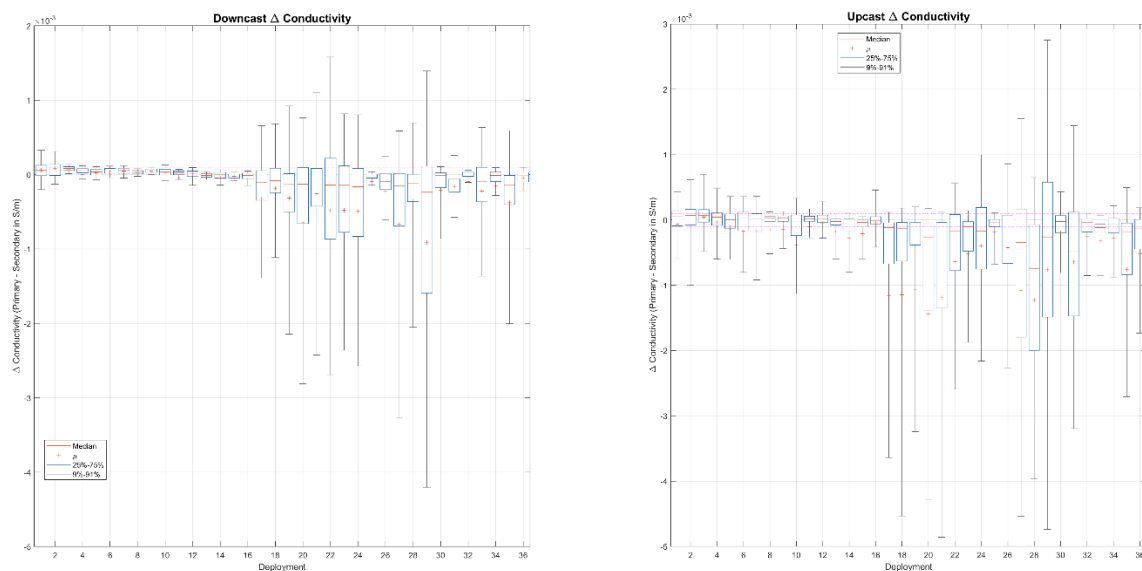


Figure 5 Difference between primary and secondary conductivity sensors

The final result for the primary and secondary conductivity sensors with respect to their original calibrations are shown in

Secondary	1-16, 25, 26, 30, 32-36	0.99975	0.00045424	-1.136e-5	0.0021253	0.0020069	0.0013571
-----------	-------------------------	---------	------------	-----------	-----------	-----------	-----------

Table 2 and

Secondary	1-16, 25, 26, 30, 32-36	-9.4818e-8	1.1151e-7
-----------	-------------------------	------------	-----------

Table 3.

Sensor Group	Deployments	Scale Factor		Offset		Salinity (PSU)	
		a1	±	a0	±	Residual SD	M.A.D.
Primary	1-16, 25, 26, 30, 32-36	0.99966	0.00042512	0.0006938	0.0019867	0.0019084	0.0011545
Secondary	1-16, 25, 26, 30, 32-36	0.99975	0.00045424	-1.136e-5	0.0021253	0.0020069	0.0013571

Table 2 Conductivity calibration with respect to manufacturers' calibration coefficients and post-calibration results

Conductivity Sensor	Deployments	CPcor	±
Primary	1-16, 25, 26, 30, 32-36	-9.0176e-8	1.0386e-7
Secondary	1-16, 25, 26, 30, 32-36	-9.4818e-8	1.1151e-7

Table 3 Calculated CPcor for primary and secondary compared to the manufacturer nominal value of -9.5700e-08

This is a good calibration. We normally aim for a S.D. of 0.002 PSU for 'typical' oceanographic voyages. The above calibration factors were applied to all deployments. Full plots of residuals before and after calibration are available in Conductivity Calibration Residual Plots.

Data from the primary conductivity and temperature sensors were used to produce the averaged salinities with secondary sensors included with a suffix '_2'.

3.4 Dissolved Oxygen Sensor Calibration

3.4.1 SBE calibration procedure

AN64: *SBE 43 Dissolved Oxygen Sensor - Background Information, Deployment Recommendations, and Cleaning and Storage* (Sea-Bird, 2013) describes the SBE43 as "a polarographic membrane oxygen sensor having a single output signal of 0 to +5 volts, which is proportional to the temperature-compensated current flow occurring when oxygen is reacted inside the membrane. A Sea-Bird CTD that is equipped with an SBE43 oxygen sensor records this voltage for later conversion to oxygen concentration, using a modified version of the algorithm by Owens and Millard (1985)".

Calibration involves performing a linear regression, as per AN64-2: *SBE 43 Dissolved Oxygen Sensor Calibration and Data Corrections* (Sea-Bird, 2012) to produce new estimates of the calibration coefficients *Soc* and *Voffset*. These new coefficients are used, along with the other, manufacturer-supplied coefficients, to derive oxygen concentrations from the sensor voltages.

3.4.2 Results

Deeper casts (>1000m) are known to be affected by pressure-induced hysteresis with this sensor. This is corrected automatically within CapPro using the method discussed in AN64-3: *SBE 43 Dissolved Oxygen (DO) Sensor - Hysteresis Corrections* (Sea-Bird, 2014).

There is a small mismatch between downcast and upcast dissolved oxygen due to the response time of the sensor. No correction for the sensor lag effect has been applied.

A single calibration group was used with the associated SBE43 up-cast data to compute the new *Soc* and *Voffset* coefficients. The plot below is of CTD - bottle oxygen differences for both upcast and downcast data (red indicates 'bad' data; + for upcast and square for downcast).

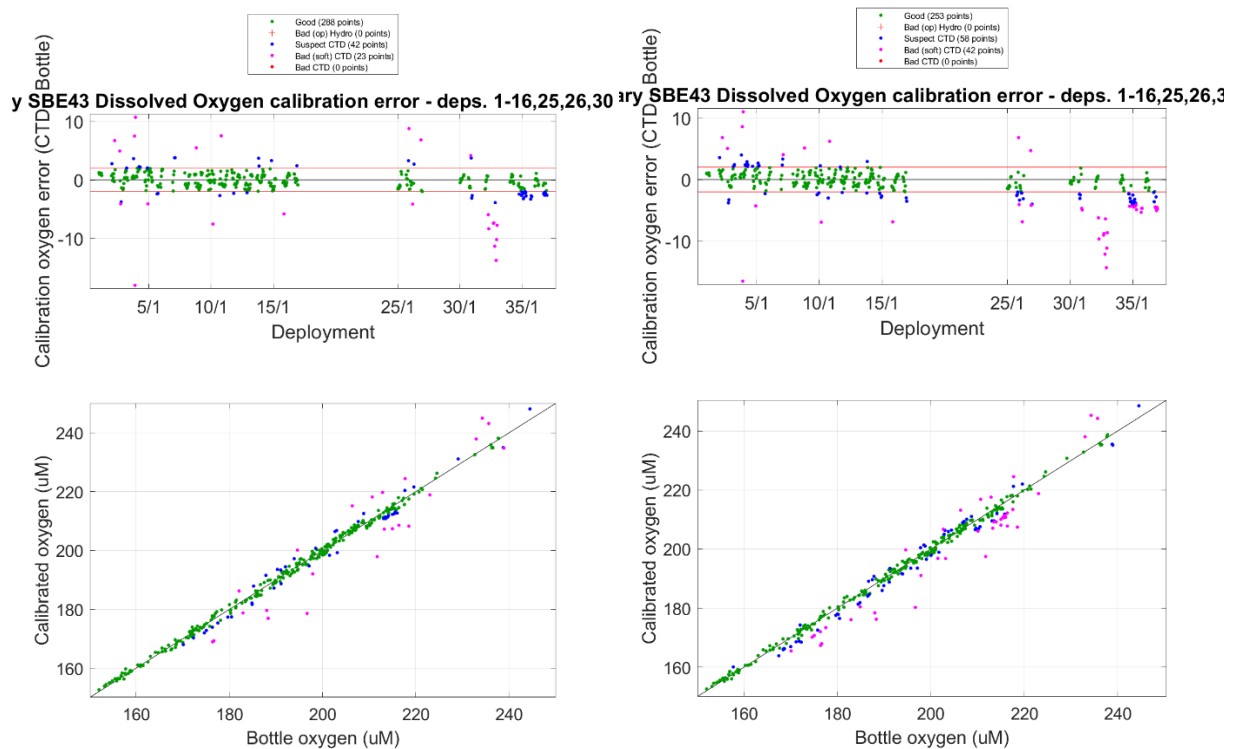


Figure 6 Dissolved Oxygen Difference with upcast CTD data (SBE43 - Bottle)

The box plot of calibrated downcast Dissolved Oxygen readings (primary - secondary) at the bottle sampling depths for all deployments in Figure 7 shows that the calibrated Dissolved Oxygen sensor responses corresponded well.

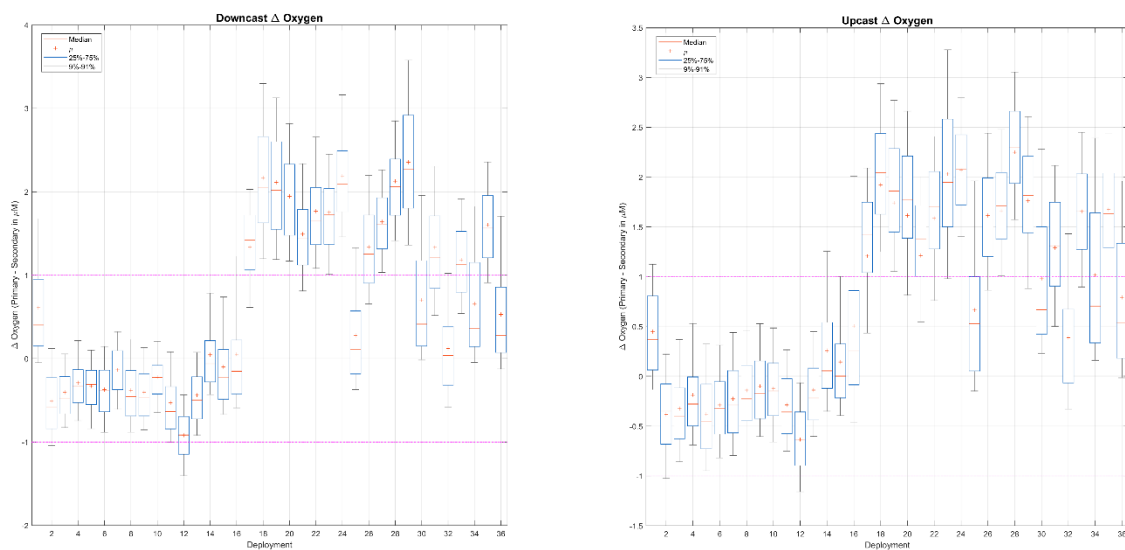


Figure 7 Difference between primary and secondary Dissolved Oxygen sensors

The old and new *Soc* and *Voffset* values for DO sensors are listed in Table 2 below. The *Soc* value is a linear slope scaling coefficient; *Voffset* is the fixed sensor voltage at zero oxygen. As expected, over time, the increasing *Soc* scale factors show the SBE43 sensor is losing sensitivity. Full plots of residuals before and after calibration are available in Dissolved Oxygen Calibration Residual Plots.

The calibrations were applied for each sensor and the averaged files were created using the result from the primary sensor.

Sensor	Calibration Source	Deployments	Calibration Coefficients				Dissolved Oxygen (μM)	
			<i>Voffset</i>	\pm	<i>Soc</i>	\pm	Residual SD	M.A.D.
Primary DO	CapPro	1-16, 25, 26, 30, 32-36	-0.49411	0.001867	0.54194	0.00094545	0.84461	0.97214
	CSIRO Cal Lab	1-36	-0.50539		0.52968			
Secondary DO	CapPro	1-16, 25, 26, 30, 32-36	-0.47306	0.0022034	0.50662	0.00099397	0.95217	0.9929
	Sea-Bird	1-36	-0.47500		0.47800			

Figure 7 Dissolved oxygen calibrations

3.5 Other sensors

The C-Star transmissometer was used on all deployments. It was calibrated by the manufacturer with meter outputs with the beam blocked, in air with a clear beam path and with clean water in the path. These values are used to determine a scale and offset for use in SBE Data Processing software to convert the raw counts to a beam transmittance output of 0-100 percent.

The WET labs ECO Fluorometer-Scattering sensor was used for all deployments. The fluorometer has been calibrated with manufacturer supplied coefficients to give outputs in mg/m³. The scattering (OBS) has been calibrated with manufacturer supplied coefficients to give outputs in m⁻¹/sr.

The Biospherical PAR sensor was also used for all deployments. The output is a nominal 0-5 volts which is converted to the unit $\mu\text{Einsteins}/\text{m}^2/\text{second}$ using manufacturer supplied wet calibration factor and the dark voltage determined at calibration. This data channel has been included in the output files for all deployments. Clearly, time of day and environmental factors such as sea state and cloud cover impact on these readings. If most or all of the values for a deployment are near zero it indicates a night-time cast. In deployments where the PAR profiles have sub-surface maxima the CTD may have been shaded by the ship.

3.6 Bad data detection

The limits for each sensor are configured in CNV_to_Scan conversion software and are written to the NetCDF scan file. Typical limits used for the sensor range and maximum second difference are in Table 4 below. The rejection rate is recorded in the CapPro processing log file.

Sensor	Units	Range minimum	Range maximum	Maximum Second Difference
Pressure	decibar	-7	6500	0.5
Temperature	degC	-10	40	0.05
Conductivity	S/m	-0.01	7	0.01
Oxygen	μM	-0.1	500	0.5

Fluorometer	mg/m ³	0	30	0.5
PAR	μE/m ² /sec	-5	5000	0.5
Transmissometer	%	0	100	0.5
OBS	m ⁻¹ /sr	0	0.0008	0.5
CDOM	ppb	-5	515	0.5
Altimeter	m	0	50	0.5

Table 4 Sensor limits for bad data detection

3.7 Heave Filtering

Sensor data impacted by ship heave impeding the CTD deployment is filtered out in three stages, and applied during data binning. The first stage detects negative acceleration of the CTD which can cause trailing mixed water to be pumped through the sensors. The second stage looks at all negative density gradients and flags readings which are above 10 times the standard deviation of all negative gradients, for 2 seconds. The third stage flags any pressure reversals which are greater than the height of the CTD sensor pump inlet above the frame.

3.8 Averaging

The calibrated data were 'filtered' to remove pressure reversals and binned into the standard product of 1 decibar averaged NetCDF files. The binned values were calculated by applying a linear, least-squares fit as a function of pressure to the sensor data for each bin, using this to interpolate the value for the bin mid-point. This method is used to avoid possible biases which would result from averaging with respect to time.

Each binned parameter is assigned a QC flag. Our quality control flagging scheme is described in *Data Quality Control Flags* (Pender, 2000).


The QC Flag for each bin is estimated from the values for the bin components. The QC Flag for derived quantities, such as Salinity and Dissolved Oxygen are taken to be the worst of the estimates for the parameters from which they are derived.

4 References




- Chris Chapman. (2021). *The RV Investigator. Voyage Plan in2021_v03*. Retrieved from Marine National Facility: Voyage Plans and summaries: <http://mnf.csiro.au/Voyages/Investigator-schedules/Plans-and-summaries/>
- Pender, L. (2000). *Data Quality Control Flags*. Retrieved from Oceans & Atmosphere Information and Data Centre: http://www.cmar.csiro.au/datacentre/ext_docs/DataQualityControlFlags.pdf
- Sea-Bird. (2012). *AN64-2: SBE 43 Dissolved Oxygen Sensor Calibration and Data Corrections*. Retrieved from Sea-Bird Electronics: <https://www.seabird.com/asset-get.download.jsa?code=251034>
- Sea-Bird. (2013). *AN64: SBE 43 Dissolved Oxygen Sensor - Background Information, Deployment Recommendations, and Cleaning and Storage*. Retrieved from Sea-Bird Electronics: <https://www.seabird.com/asset-get.download.jsa?code=251036>
- Sea-Bird. (2014). *AN64-3: SBE 43 Dissolved Oxygen (DO) Sensor - Hysteresis Corrections*. Retrieved from Sea-Bird Electronics: <https://www.seabird.com/asset-get.download.jsa?code=251035>

Appendix I: Conductivity Calibration Residual Plots


Primary SBE4 Conductivity residual before cal. 1-16,25,26,30,32,34-3

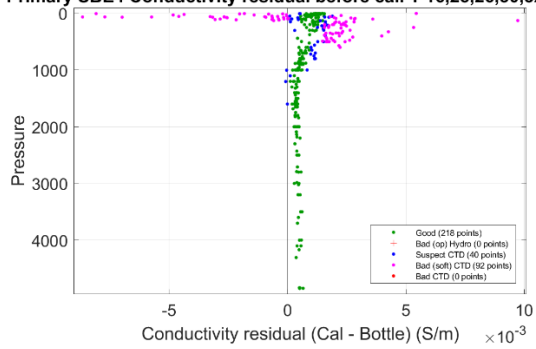




Primary SBE4 Conductivity residual after cal. 1-16,25,26,30,32,34-3

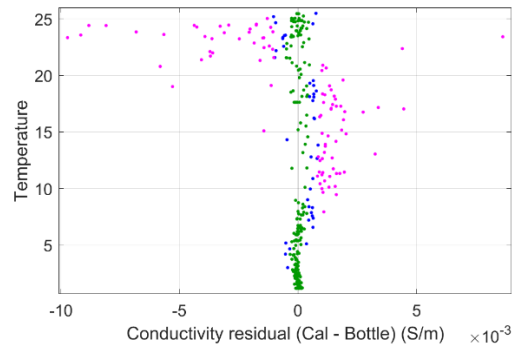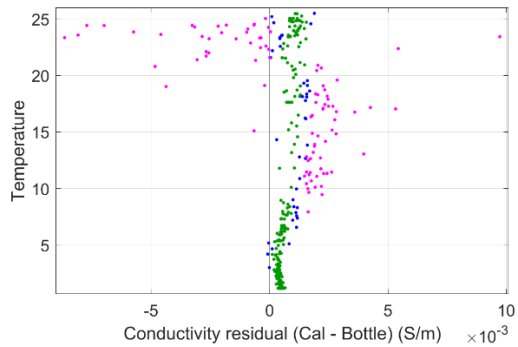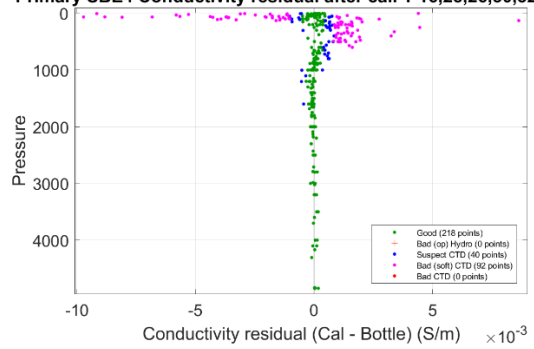

Secondary SBE4 Conductivity residual before cal. 1-16,25,26,30,32,34

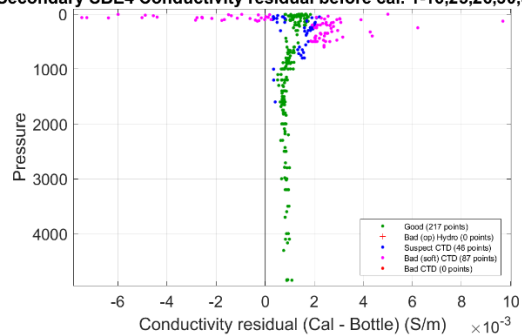


Secondary SBE4 Conductivity residual after cal. 1-16,25,26,30,32,34

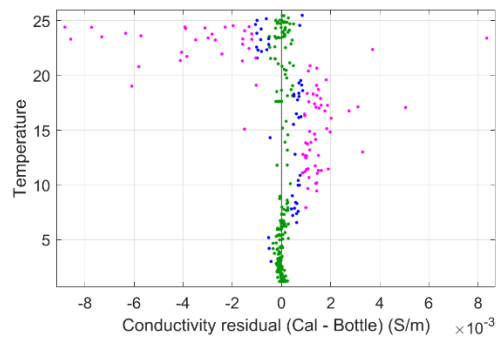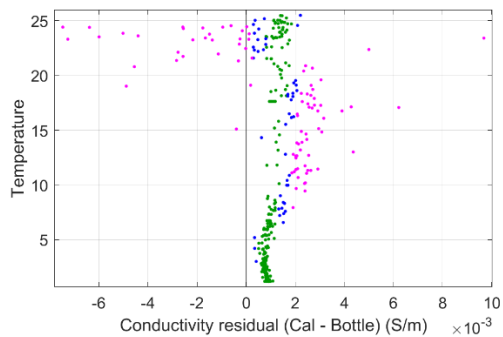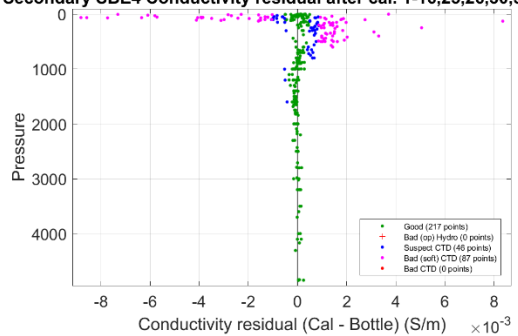

Appendix II: Dissolved Oxygen Calibration Residual Plots

Primary SBE43 Dissolved Oxygen residual before cal. 1-16,25,26,30,32, Primary SBE43 Dissolved Oxygen residual after cal. 1-16,25,26,30,32,3

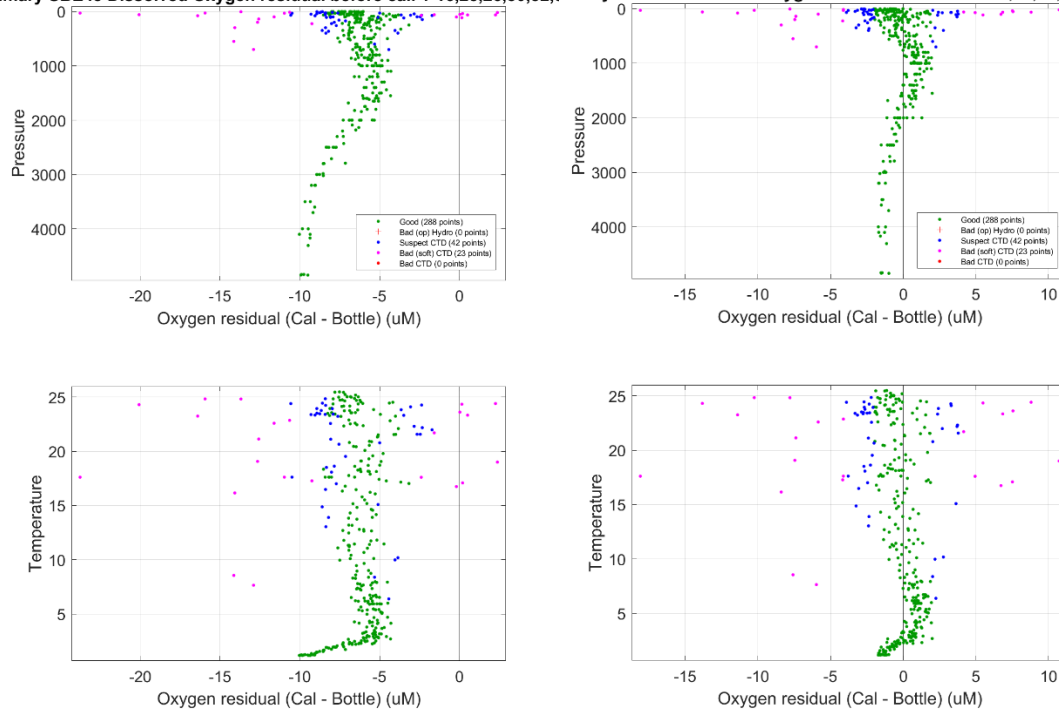

Secondary SBE43 Dissolved Oxygen residual before cal. 1-16,25,26,30,32, Secondary SBE43 Dissolved Oxygen residual after cal. 1-16,25,26,30,32,

