


## *RV Investigator*

### CTD Processing Report

<b>Voyage ID:</b>	IN2021_T01
<b>Voyage title:</b>	Transit: Brisbane to Darwin
<b>Depart:</b>	Brisbane, 1800 Wednesday, 9 June 2021
<b>Return:</b>	Darwin, 0900 Wednesday, 23 June 2021

### Document History

Date	Version	Author	Comments
21 /07/2021	1.0	David Webb	Initial version

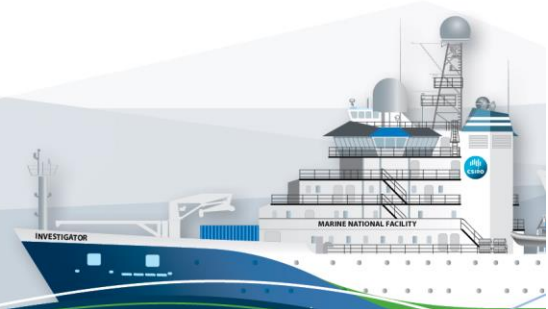

## Contents

1	Summary .....	3
2	Voyage Details .....	3
2.1	Title.....	3
2.2	Principal Investigators .....	3
2.3	Voyage Objectives .....	3
2.4	Area of operation .....	4
3	Processing Notes.....	5
3.1	Background Information.....	5
3.2	Pressure and temperature calibration .....	6
3.3	Conductivity Calibration .....	7
3.4	Dissolved Oxygen Sensor Calibration .....	10
3.4.1	SBE calibration procedure .....	10
3.4.2	Results.....	10
3.5	Other sensors .....	12
3.6	Bad data detection .....	12
3.7	Heave Filtering .....	12
3.8	Averaging.....	12
4	References .....	13
	Appendix I: Conductivity Calibration Residual Plots.....	14
	Appendix II: Dissolved Oxygen Calibration Residual Plots .....	15

# 1 Summary

These notes relate to the production of quality controlled, calibrated CTD data from RV Investigator voyage IN2021\_T01, from 09 Jun 2021 – 23 Jun 2021.

Data for 12 deployments were acquired using the Sea-Bird SBE911 CTD #24, fitted with 36 twelve litre bottles on the rosette sampler. Sea-Bird-supplied calibration factors were used to compute the pressures and preliminary conductivity values. CSIRO -supplied calibrations were applied to the temperature data. The data were subjected to automated QC to remove spikes and out-of-range values.

The final conductivity calibration was based on a single deployment grouping. The final calibration from the primary sensor had a standard deviation (SD) of 0.0033235 PSU, outside our target of 'better than 0.002 PSU'. The standard product of 1 decibar binned averaged were produced using data from the primary sensors.

The dissolved oxygen data calibration fit had a SD of 0.64275  $\mu\text{M}$ . The agreement between the CTD and bottle data was good.

PAR, upward and downward facing Teledyne Lowered Acoustic Doppler Current Profilers (LADCP), Wetlabs C-Star Transmissometer, ECO Chlorophyll and Scattering, CDOM, and UBAT sensors were also installed on the auxiliary A/D channels of the CTD.

## 2 Voyage Details

### 2.1 Title

Transit: Brisbane to Darwin

### 2.2 Principal Investigators


Viena Puigcorb  (Edith Cowan University)

### 2.3 Voyage Objectives

The scientific objectives for IN2021\_T01 were outlined in the Voyage Plan.

For further details, refer to the Voyage Plan and/or summary which can be viewed on the Marine National Facility web site.

## 2.4 Area of operation

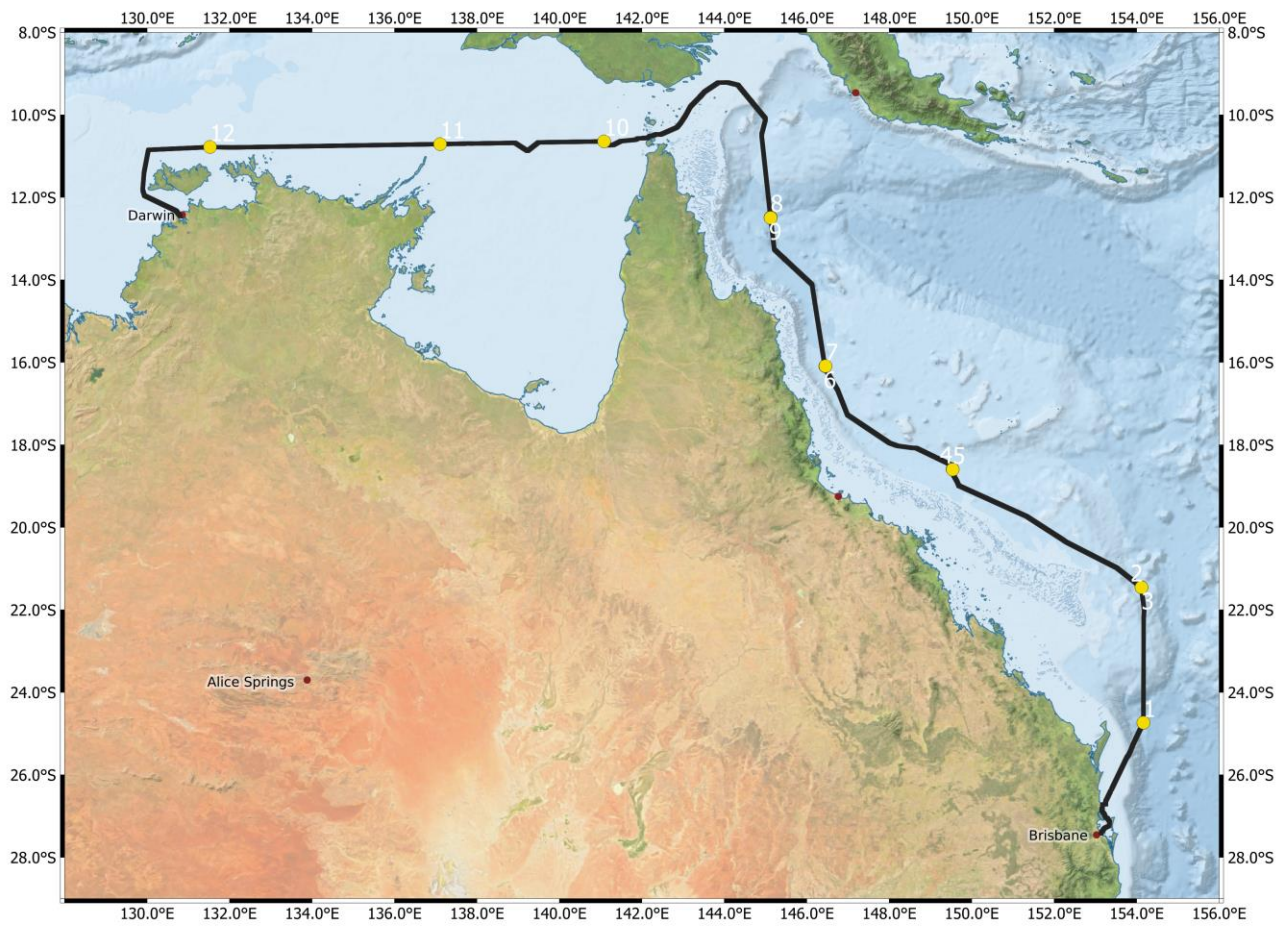

**Figure 1 Area of operation for IN2021\_T01**

## 3 Processing Notes

### 3.1 Background Information

The data for this voyage were acquired with the CSIRO CTD unit #24, a Sea-Bird SBE911 with dual conductivity and temperature sensors.

The CTD was additionally fitted with SBE43 dissolved oxygen sensors, altimeter, PAR, upward and downward facing Teledyne Lowered Acoustic Doppler Current Profilers (LADCP), Wetlabs ECO Chlorophyll and Scattering, CDOM, C-Star Transmissometer, and UBAT sensors. These sensors are described in

PAR	Biospherical QCP2300HP	70111	A3	20-Oct-2020	Chelsea
Transmissometer	Wetlabs C-Star	CST-2009DR	A4	28-Oct-2020	Sea-Bird Wetlabs
CDOM	Wetlabs FLCDRD	4367	A5	18-May-2020	Sea-Bird Wetlabs
Wetlabs ECO - Chlorophyll	FLBB	5169	A6	16-Nov-2020	Sea-Bird Wetlabs
Wetlabs ECO - Scattering	FLBB	5169	A7	16-Nov-2020	Sea-Bird Wetlabs
Wetlabs UBAT	UBAT	0041	Serial uplink	-	-
LADCP Upward Facing	Teledyne 300kHz	24502	Internal	-	-
LADCP Downward Facing	Teledyne 150kHz	24638	Internal	-	-
LADCP Battery	OceanDeep	2219	-	-	-

Table 1 below.

Description	Model	Serial No.	A/D	Calibration Date	Calibration Source
CTD #24	SBE9+ V2	1332	-	-	-
Primary Temperature	SBE3T	6180	T0	23-Jan-2021	CSIRO
Secondary Temperature	SBE3T	6285	T1	25-Sep-2020	CSIRO
Primary Conductivity	SBE4C	4773	C0	21-Sep-2020	CSIRO
Secondary Conductivity	SBE4C	4774	C1	21-Sep-2020	CSIRO
Primary Dissolved Oxygen	SBE43	3155	A0	14-Oct-2020	CSIRO
Secondary Dissolved Oxygen	SBE43	1794	A1	21-Nov-2020	Sea-Bird
Altimeter	Tritech PA500	228403	A2	29-May-2020	Tritech
PAR	Biospherical QCP2300HP	70111	A3	20-Oct-2020	Chelsea
Transmissometer	Wetlabs C-Star	CST-2009DR	A4	28-Oct-2020	Sea-Bird Wetlabs
CDOM	Wetlabs FLCDRD	4367	A5	18-May-2020	Sea-Bird Wetlabs
Wetlabs ECO - Chlorophyll	FLBB	5169	A6	16-Nov-2020	Sea-Bird Wetlabs
Wetlabs ECO - Scattering	FLBB	5169	A7	16-Nov-2020	Sea-Bird Wetlabs
Wetlabs UBAT	UBAT	0041	Serial uplink	-	-
LADCP Upward Facing	Teledyne 300kHz	24502	Internal	-	-
LADCP Downward Facing	Teledyne 150kHz	24638	Internal	-	-
LADCP Battery	OceanDeep	2219	-	-	-

**Table 1 CTD Sensor configuration on IN2021\_T01**

Water samples were collected using a Sea-Bird SBE32, 36-bottle rosette sampler. Sampling was from 36 twelve litre bottles which were fitted to the frame.


The raw CTD data were collected in SBE SeaSave version 7.26.7.110, converted to scientific units using SBE Data Processing version 7.26.7 and written to NetCDF format files with CNV\_to\_Scan for processing using the Matlab-base, CapPro package version 2.11.

The CapPro software was used to apply automated QC and preliminary processing to the data. This included spike removal, identification of water entry and exit times, conductivity sensor lag corrections, conductivity cell thermal inertia corrections, and the determination of the pressure offsets. It also loaded the hydrology data and computed the matching CTD sample burst data. The automatically determined pressure offsets and in-water points were inspected.

The bottle sample data were used to compute final conductivity and dissolved oxygen calibrations. These were applied to the data, after which files of binned 1 decibar averaged data were produced.


### **3.2 Pressure and temperature calibration**

The pressure offsets are plotted in Figure 2 below. The blue circles refer to initial out-of-water values and the red circles the final out-of-water values.

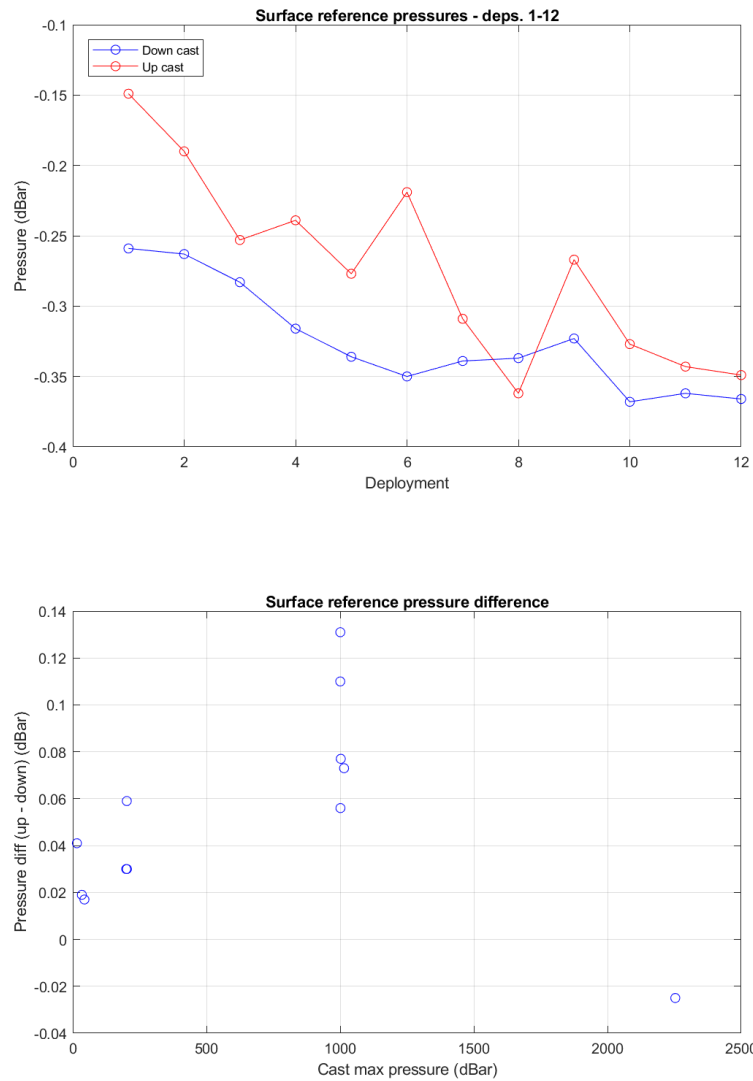

**Figure 2 CTD pressure offsets**

The difference between the primary and secondary temperature sensors at the bottle sampling depths is plotted below. Most deployments plot within  $\pm 0.001^{\circ}\text{C}$  of zero – outliers result from sampling in regions of high vertical temperature gradient as supported by the similarity between the temperature and conductivity difference shown in Figure 3. This indicates neither sensor has drifted significantly from its calibration.

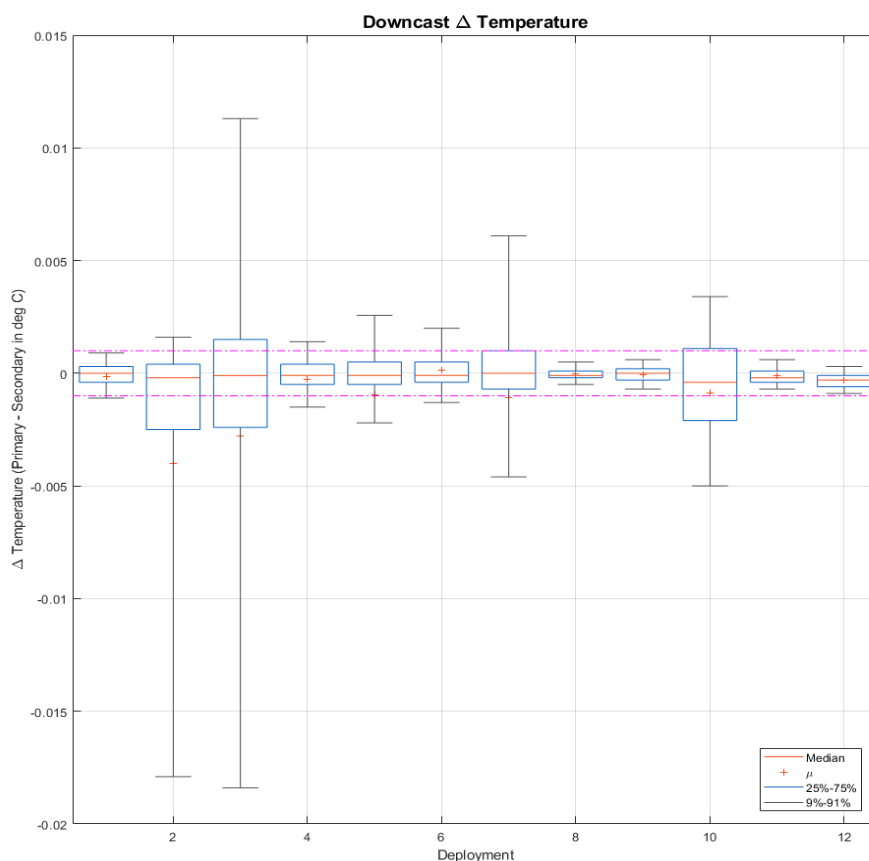


**Figure 3** *Difference between primary and secondary temperature sensors*

### 3.3 Conductivity Calibration

Discrepancies and possible sampling problems between bottle and CTD salinities for the primary conductivity sensor would show in Figure 4; the plot of calibrated (CTD - Bottle) salinity below. The calibration was based upon the sample data (primary/secondary) for 5/0 of the total of 5 samples taken during deployments which are above our target of 70%.


The outliers marked in Figure 4 below with magenta dots are excluded from the calibration, the outliers marked with blue dots are used in the calibration but are weighted based on their distance from the mean. Any outliers marked with red crosses or dots are also excluded from the calibration.



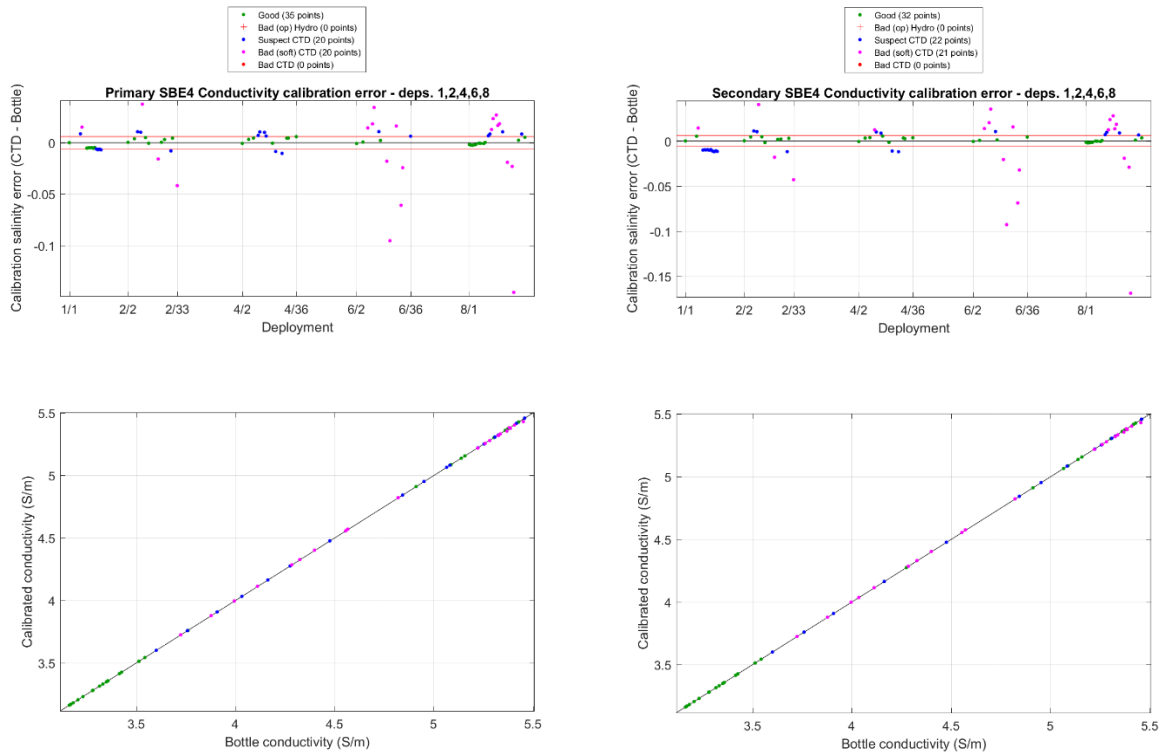

**Figure 4 CTD - bottle salinity plot**

The box plot of calibrated downcast conductivities (primary - secondary) at the bottle sampling depths for all deployments in Figure 5 shows that the calibrated conductivity cell responses corresponded very well.

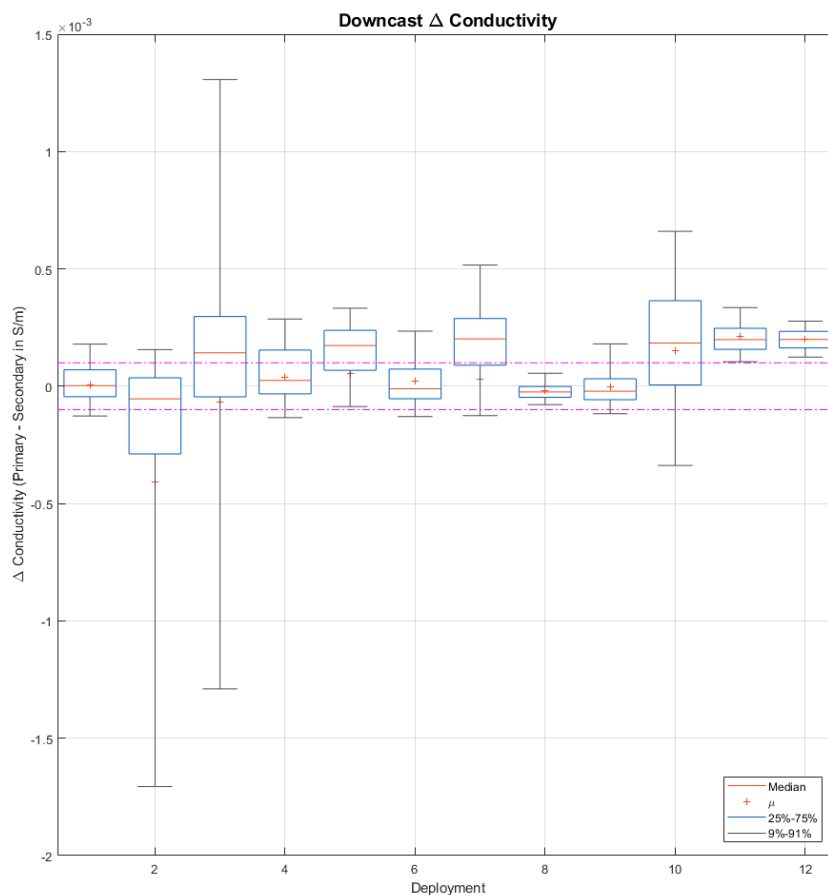

**Figure 5 Difference between primary and secondary conductivity sensors**

The final result for the primary and secondary conductivity sensors with respect to their original calibrations are shown in

Secondary	1,2,4,6,8	0.99992	0.0041323	-0.00039145	0.021716	0.0042317	0.0039897
-----------	-----------	---------	-----------	-------------	----------	-----------	-----------

Table 2 and

Secondary	1,2,4,6,8	-5.9699e-08	2.3035e-06
-----------	-----------	-------------	------------

Table 3.

Sensor Group	Deployments	Scale Factor		Offset		Salinity (PSU)	
		a1	±	a0	±	Residual SD	M.A.D.
Primary	1,2,4,6,8	1	0.0036497	-0.00040297	0.019156	0.0033235	0.0047508
Secondary	1,2,4,6,8	0.99992	0.0041323	-0.00039145	0.021716	0.0042317	0.0039897

**Table 2 Conductivity calibration with respect to manufacturers' calibration coefficients and post-calibration results**

Conductivity Sensor	Deployments	CPcor	±
Primary	1,2,4,6,8	-6.5592e-08	2.0396e-06
Secondary	1,2,4,6,8	-5.9699e-08	2.3035e-06

**Table 3 Calculated CPcor for primary and secondary compared to the manufacturer nominal value of -9.5700e-08**

This is a marginal calibration. We normally aim for a S.D. of 0.002 PSU for 'typical' oceanographic voyages. The above calibration factors were applied to all deployments. Full plots of residuals before and after calibration are available in Conductivity Calibration Residual Plots. Data from the primary conductivity and temperature sensors were used to produce the averaged salinities with primary sensors included with a suffix '\_1'.

### 3.4 Dissolved Oxygen Sensor Calibration

#### 3.4.1 SBE calibration procedure

*AN64: SBE 43 Dissolved Oxygen Sensor - Background Information, Deployment Recommendations, and Cleaning and Storage* (Sea-Bird, 2013) describes the SBE43 as "a polarographic membrane oxygen sensor having a single output signal of 0 to +5 volts, which is proportional to the temperature-compensated current flow occurring when oxygen is reacted inside the membrane. A Sea-Bird CTD that is equipped with an SBE43 oxygen sensor records this voltage for later conversion to oxygen concentration, using a modified version of the algorithm by Owens and Millard (1985)".


Calibration involves performing a linear regression, as per *AN64-2: SBE 43 Dissolved Oxygen Sensor Calibration and Data Corrections* (Sea-Bird, 2012) to produce new estimates of the calibration coefficients *Soc* and *Voffset*. These new coefficients are used, along with the other, manufacturer-supplied coefficients, to derive oxygen concentrations from the sensor voltages.

#### 3.4.2 Results

Deeper casts (>1000m) are known to be affected by pressure-induced hysteresis with this sensor. This is corrected automatically within CapPro using the method discussed in *AN64-3: SBE 43 Dissolved Oxygen (DO) Sensor - Hysteresis Corrections* (Sea-Bird, 2014).


There is a small mismatch between downcast and upcast dissolved oxygen due to the response time of the sensor. No correction for the sensor lag effect has been applied.

A single calibration group was used with the associated SBE43 up-cast data to compute the new *Soc* and *Voffset* coefficients. The plot below is of CTD - bottle oxygen differences for both upcast and downcast data (red indicates 'bad' data; + for upcast and square for downcast).

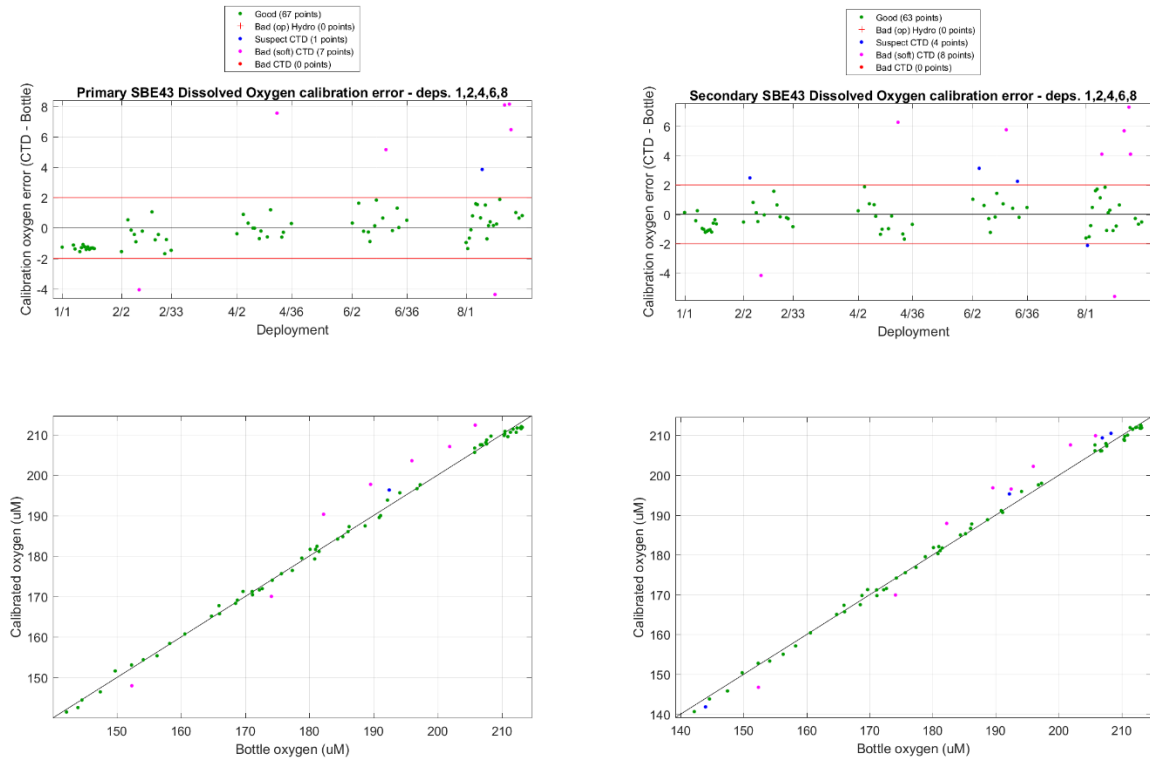

**Figure 6 Dissolved Oxygen Difference with upcast CTD data (SBE43 - Bottle)**

The box plot of calibrated downcast Dissolved Oxygen readings (primary - secondary) at the bottle sampling depths for all deployments in Figure 7 shows that the calibrated Dissolved Oxygen sensor responses corresponded well, except for Deployments 10-12 where the max pressure of the CTD casts were less than 50 dBar.

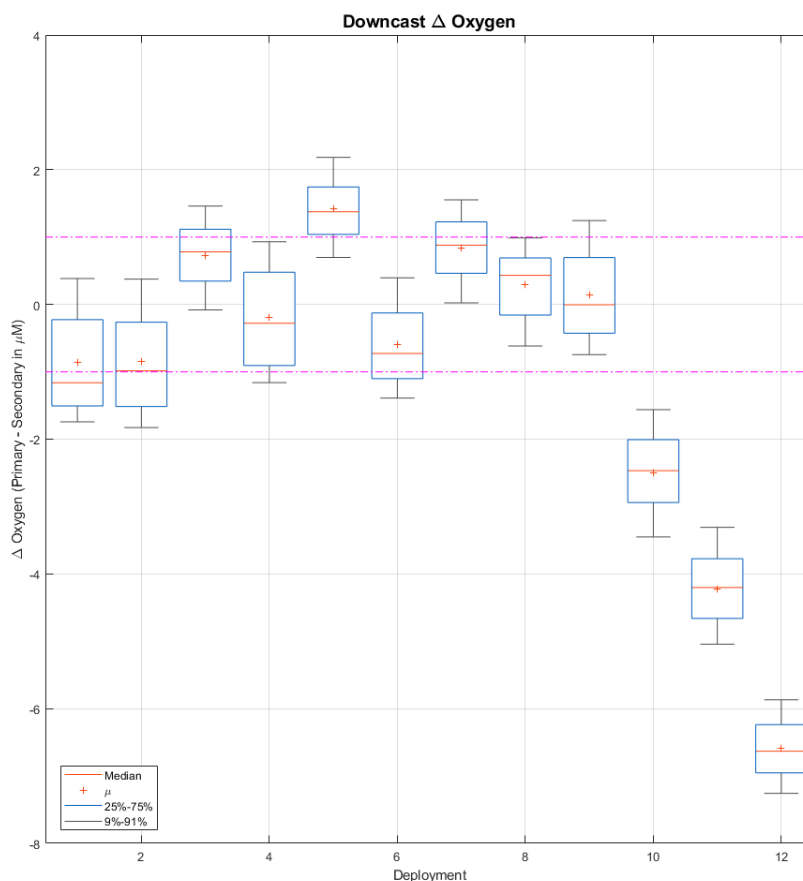

**Figure 7 Difference between primary and secondary Dissolved Oxygen sensors**

The old and new *Soc* and *Voffset* values for DO sensors are listed in Table 2 below. The *Soc* value is a linear slope scaling coefficient; *Voffset* is the fixed sensor voltage at zero oxygen. As expected, over time, the increasing *Soc* scale factors show the SBE43 sensor is losing sensitivity. Full plots of residuals before and after calibration are available in Dissolved Oxygen Calibration Residual Plots.

The calibrations were applied for each sensor and the averaged files were created using the result from the primary sensor.

Sensor	Calibration Source	Deployments	Calibration Coefficients				Dissolved Oxygen (μM)	
			<i>Voffset</i>	±	<i>Soc</i>	±	Residual SD	M.A.D.
Primary DO	CapPro	1,2,4,6,8	-0.50028	0.0046238	0.543	0.0019563	0.64275	0.78865
	CSIRO	1,2,4,6,8	-0.50830889		0.52179013			
Secondary DO	CapPro	1,2,4,6,8	-0.49057	0.0050216	0.51352	0.0018825	0.644	0.7161
	Sea-Bird	1,2,4,6,8	-0.4750		0.4780			

**Figure 7 Dissolved oxygen calibrations**

### 3.5 Other sensors

The C-Star transmissometer was used on all deployments. It was calibrated by the manufacturer with meter outputs with the beam blocked, in air with a clear beam path and with clean water in the path. These values are used to determine a scale and offset for use in SBE Data Processing software to convert the raw counts to a beam transmittance output of 0-100 percent.

The WET labs ECO Fluorometer-Scattering sensor was used for all deployments. The fluorometer has been calibrated with manufacturer supplied coefficients to give outputs in mg/m<sup>3</sup>. The scattering (OBS) has been calibrated with manufacturer supplied coefficients to give outputs in m<sup>-1</sup>/sr.

The Biospherical PAR sensor was also used for all deployments. The output is a nominal 0-5 volts which is converted to the unit  $\mu\text{Einstein}/\text{m}^2/\text{second}$  using manufacturer supplied wet calibration factor and the dark voltage determined at calibration. This data channel has been included in the output files for all deployments. Clearly, time of day and environmental factors such as sea state and cloud cover impact on these readings. If most or all of the values for a deployment are near zero it indicates a night-time cast. In deployments where the PAR profiles have sub-surface maxima the CTD may have been shaded by the ship.

### 3.6 Bad data detection

The limits for each sensor are configured in CNV\_to\_Scan conversion software and are written to the NetCDF scan file. Typical limits used for the sensor range and maximum second difference are in Table 4 below. The rejection rate is recorded in the CapPro processing log file.

Sensor	Range minimum	Range maximum	Maximum Second Difference
Pressure	-7	6500	0.5
Temperature	-2	40	0.05
Conductivity	-0.01	7	0.01
Oxygen	-1	500	0.5
Fluorometer	0	100	0.5
PAR	-5	2000	0.5
Transmissometer	0	100	0.5

*Table 4 Sensor limits for bad data detection*

### 3.7 Heave Filtering

Sensor data impacted by ship heave impeding the CTD deployment is filtered out in three stages, and applied during data binning. The first stage detects negative acceleration of the CTD which can cause trailing mixed water to be pumped through the sensors. The second stage looks at all negative density gradients and flags readings which are above 10 times the standard deviation of all negative gradients, for 2 seconds. The third stage flags any pressure reversals which are greater than the height of the CTD sensor pump inlet above the frame.

### 3.8 Averaging

The calibrated data were 'filtered' to remove pressure reversals and binned into the standard product of 1 decibar averaged NetCDF files. The binned values were calculated by applying a linear, least-squares fit as a function of pressure to the sensor data for each bin, using this to interpolate the value for the bin mid-point. This method is used to avoid possible biases which would result from averaging with respect to time.


Each binned parameter is assigned a QC flag. Our quality control flagging scheme is described in *Data Quality Control Flags* (Pender, 2000).

The QC Flag for each bin is estimated from the values for the bin components. The QC Flag for derived quantities, such as Salinity and Dissolved Oxygen are taken to be the worst of the estimates for the parameters from which they are derived.

## 4 References

- Viena Puigcorbé. (2021). *The RV Investigator. Voyage Plan IN2021\_T01*. Retrieved from Marine National Facility: Voyage Plans and summaries: <http://mnf.csiro.au/Voyages/Investigator-schedules/Plans-and-summaries/>
- Pender, L. (2000). *Data Quality Control Flags*. Retrieved from Oceans & Atmosphere Information and Data Centre: [http://www.cmar.csiro.au/datacentre/ext\\_docs/DataQualityControlFlags.pdf](http://www.cmar.csiro.au/datacentre/ext_docs/DataQualityControlFlags.pdf)
- Sea-Bird. (2012). *AN64-2: SBE 43 Dissolved Oxygen Sensor Calibration and Data Corrections*. Retrieved from Sea-Bird Electronics: <https://www.seabird.com/asset-get.download.jsa?code=251034>
- Sea-Bird. (2013). *AN64: SBE 43 Dissolved Oxygen Sensor - Background Information, Deployment Recommendations, and Cleaning and Storage*. Retrieved from Sea-Bird Electronics: <https://www.seabird.com/asset-get.download.jsa?code=251036>
- Sea-Bird. (2014). *AN64-3: SBE 43 Dissolved Oxygen (DO) Sensor - Hysteresis Corrections*. Retrieved from Sea-Bird Electronics: <https://www.seabird.com/asset-get.download.jsa?code=251035>

## Appendix I: Conductivity Calibration Residual Plots

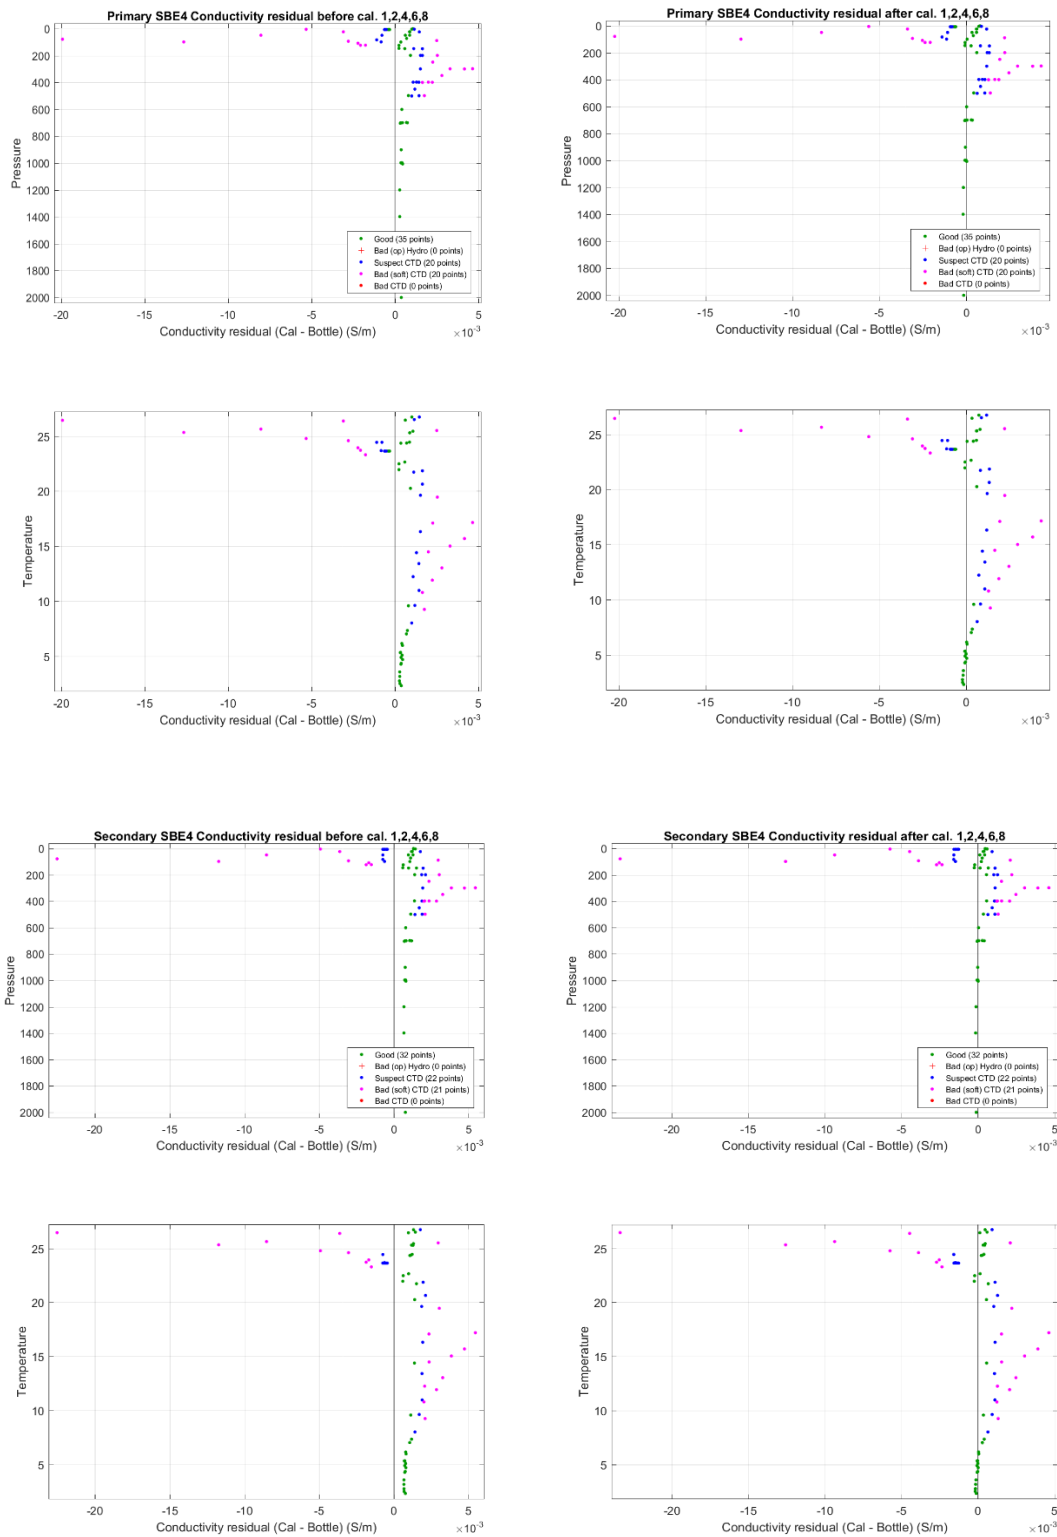



## Appendix II: Dissolved Oxygen Calibration Residual Plots

