


RV Investigator

CTD Processing Report

Voyage ID:	in2021_v04
Voyage title:	Biodiversity Assessment of Australia's Indian Ocean Territories
Depart:	Darwin, 0830 ACST Wednesday, 30 th June 2021
Return:	Hobart, 1130 AEST Thursday, 29 th July 2021

Document History

Date	Version	Author	Comments
11/08/2021	1.0	Stephanie Zeliadt	Initial version

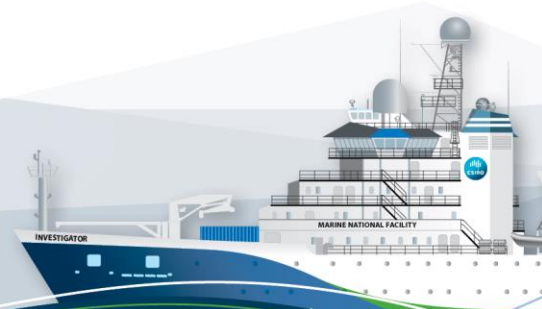

Contents

1	Summary	3
2	Voyage Details	3
2.1	Title.....	3
2.2	Principal Investigators	3
2.3	Voyage Objectives	3
2.4	Area of operation	4
3	Processing Notes.....	5
3.1	Background Information	5
3.2	Pressure and temperature calibration.....	6
3.3	Conductivity Calibration.....	8
3.4	Dissolved Oxygen Sensor Calibration	11
3.4.1	SBE calibration procedure	11
3.4.2	Results	11
3.5	Other sensors.....	13
3.6	Bad data detection.....	13
3.7	Heave Filtering.....	14
3.8	Averaging	14
4	References.....	15
	Appendix I: Conductivity Calibration Residual Plots	16
	Appendix II: Dissolved Oxygen Calibration Residual Plots	17

1 Summary

These notes relate to the production of quality controlled, calibrated CTD data from RV Investigator voyage in2021_v04, from 30 Jun 2021 – 29 Jul 2021.

Data for 25 deployments were acquired using the Sea-Bird SBE911 CTD 24, fitted with 36 twelve litre bottles on the rosette sampler. Sea-Bird-supplied calibration factors were used to compute the pressures and preliminary conductivity values. CSIRO-supplied calibrations were applied to the temperature data. The data were subjected to automated QC to remove spikes and out-of-range values.

The final conductivity calibration was based on a single deployment grouping. The final calibration from the primary sensor had a standard deviation (SD) of 0.0013062 PSU, within our target of 'better than 0.002 PSU'. The standard product of 1 decibar binned averaged were produced using data from the primary sensors.

The dissolved oxygen data calibration fit had a SD of 0.089089µM. The agreement between the CTD and bottle data was good.

There was an observed spike in values indicating a blockage in the secondary sensors of CTD deployment 11 around 2700 decibar and it is recommended to use the primary sensor data.

An Altimeter, Nephelometer, Transmissometer, CDOM, Fluorometer, and Turbidity meter were also installed on the auxiliary A/D channels of the CTD. The Seapoint nephelometer values were found to be out of the expected range for the sensor.

2 Voyage Details

2.1 Title

Biodiversity Assessment of Australia's Indian Ocean Territories

2.2 Principal Investigators

Tim O'Hara, Museum Victoria

2.3 Voyage Objectives

The scientific objectives for in2021_v04 were outlined in the Voyage Plan.

For further details, refer to the Voyage Plan and/or summary which can be viewed on the Marine National Facility web site.

2.4 Area of operation

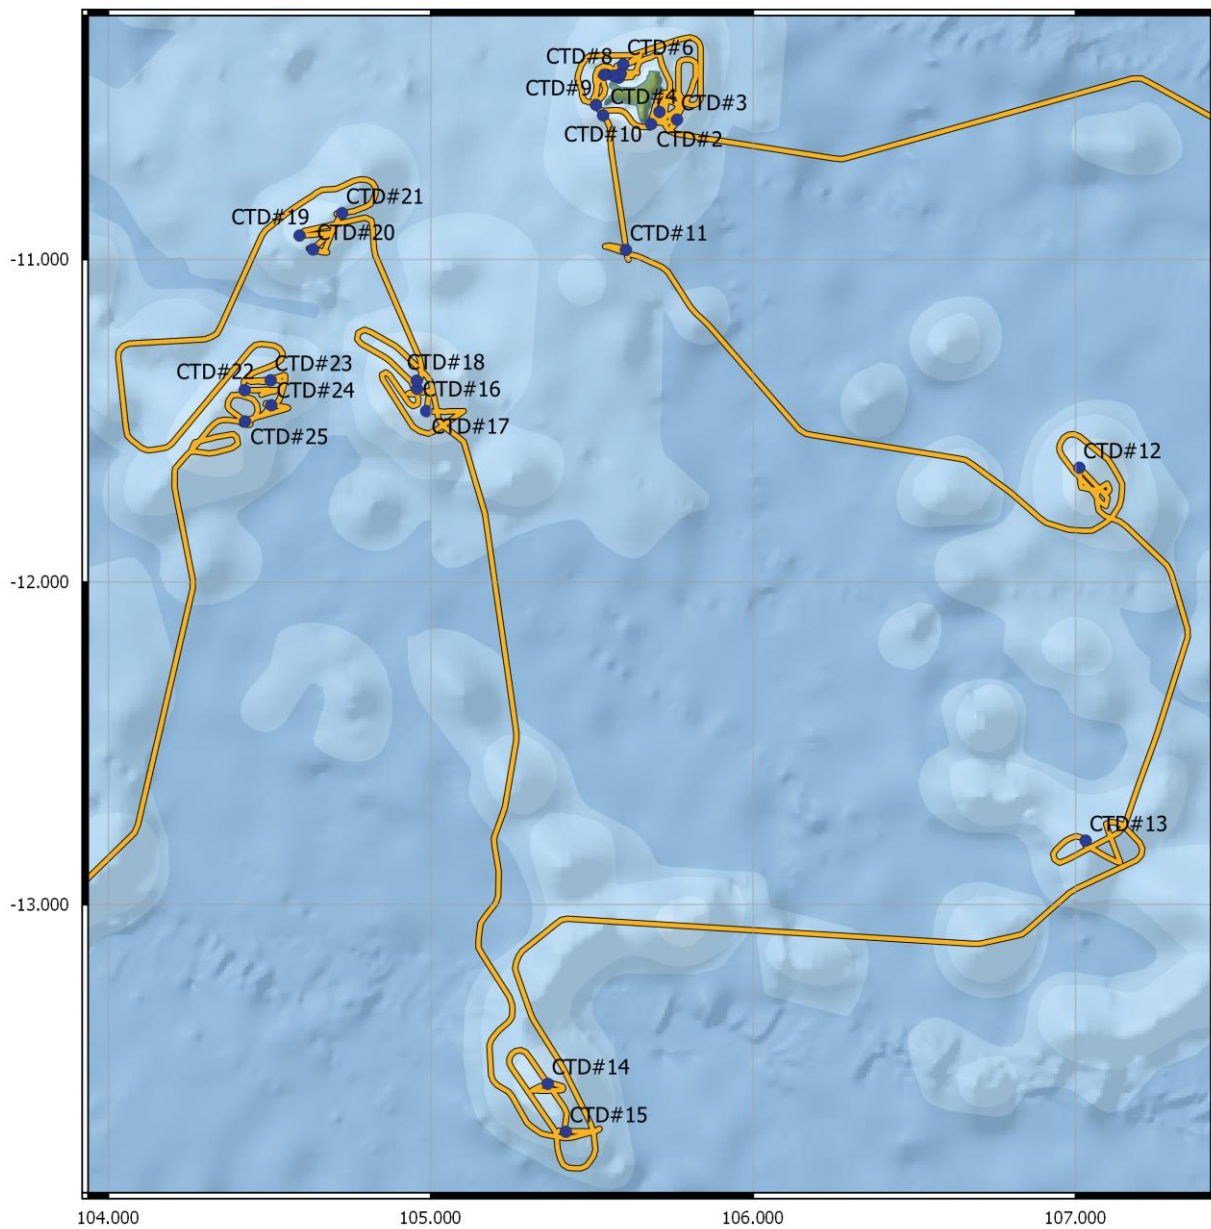


Figure 1 Area of operation for in2021_v04

3 Processing Notes

3.1 Background Information

The data for this voyage were acquired with the CSIRO CTD unit 24, a Sea-Bird SBE911 with dual conductivity and temperature sensors.

The CTD was additionally fitted with SBE43 dissolved oxygen sensors, an Altimeter, Nephelometer, Transmissometer, CDOM, Fluorometer, and Turbidity meter. These sensors are described in Table 1 below.

Description	Sensor	Serial No.	A/D	Calibration Date	Calibration Source
Pressure	Digiquartz 410K-134	1332	P	2-Jul-2020	CSIRO Cal Lab
Primary Temperature	Sea-Bird SBE3T	6180	T0	23-Jan-2021	CSIRO Cal Lab
Secondary Temperature	Sea-Bird SBE3T	6285	T1	25-Sep-2020	CSIRO Cal Lab
Primary Conductivity	Sea-Bird SBE4C	4773	C0	21-Sep-2021	CSIRO Cal Lab
Secondary Conductivity	Sea-Bird SBE4C	4774	C1	21-Sep-2020	CSIRO Cal Lab
Primary Dissolved Oxygen	SBE43	3155	A0	14-Oct-2020	CSIRO Cal Lab
Secondary Dissolved Oxygen	SBE43	1794	A1	21-Nov-2020	Sea-Bird
Altimeter	Tritech PA500	228403	A2	28-May-2020	Tritech
Turbidity Meter	Seapoint Nephelometer	13142	A3	5-Mar-2012	Manufacturer
Transmissometer	Wetlabs C-Star	CST-2009DR	A4	28-Oct-2020	Wet Labs
CDOM	Wetlabs FLCDRD	4367	A5	18-May-2020	Wet Labs
Wetlabs ECO - Chlorophyll	FLBB	5169	A6	16-Nov-2020	Wet Labs
Wetlabs ECO - Scattering	FLBB	5169	A7	16-Nov-2020	Wet Labs

Table 1 CTD Sensor configuration on in2021_v04

Water samples were collected using a Sea-Bird SBE32, 36-bottle rosette sampler. Sampling was from 36 twelve litre bottles which were fitted to the frame.

There were 25 deployments and of these, no deployments were on-deck TSG calibration runs. There was an observed spike in values indicating a blockage in the secondary sensors of CTD deployment 11 around 2700 decibar. For deployments 1-11 and 13, bottle stops were 60 seconds in duration and for 12, 14-25, the stops for the upper 500 decibar were increased to 90 seconds. The increase in bottle stop length was an attempt to reduce the amount of sensor noise at the beginning of each bottle stop at depths shallower than 500db, particularly when the salinity trace for the cast varies a lot in the top 500dbar.

The raw CTD data were collected in SBE SeaSave version 7.26.7.110, converted to scientific units using SBE Data Processing version 7.26.7.129 and written to NetCDF format files with CNV_to_Scan for processing using the Matlab-base, CapPro package version 2.11 dated 23-Aug-2019.

The CapPro software was used to apply automated QC and preliminary processing to the data. This included spike removal, identification of water entry and exit times, conductivity sensor lag corrections, conductivity cell thermal inertia corrections, and the determination of the pressure offsets. It also loaded the hydrology data and computed the matching CTD sample burst data. The automatically determined pressure offsets and in-water points were inspected.

The bottle sample data were used to compute final conductivity and dissolved oxygen calibrations. These were applied to the data, after which files of binned 1 decibar averaged data were produced.

3.2 Pressure and temperature calibration

The pressure offsets are plotted in Figure 2 below. The blue circles refer to initial out-of-water values and the red circles the final out-of-water values.

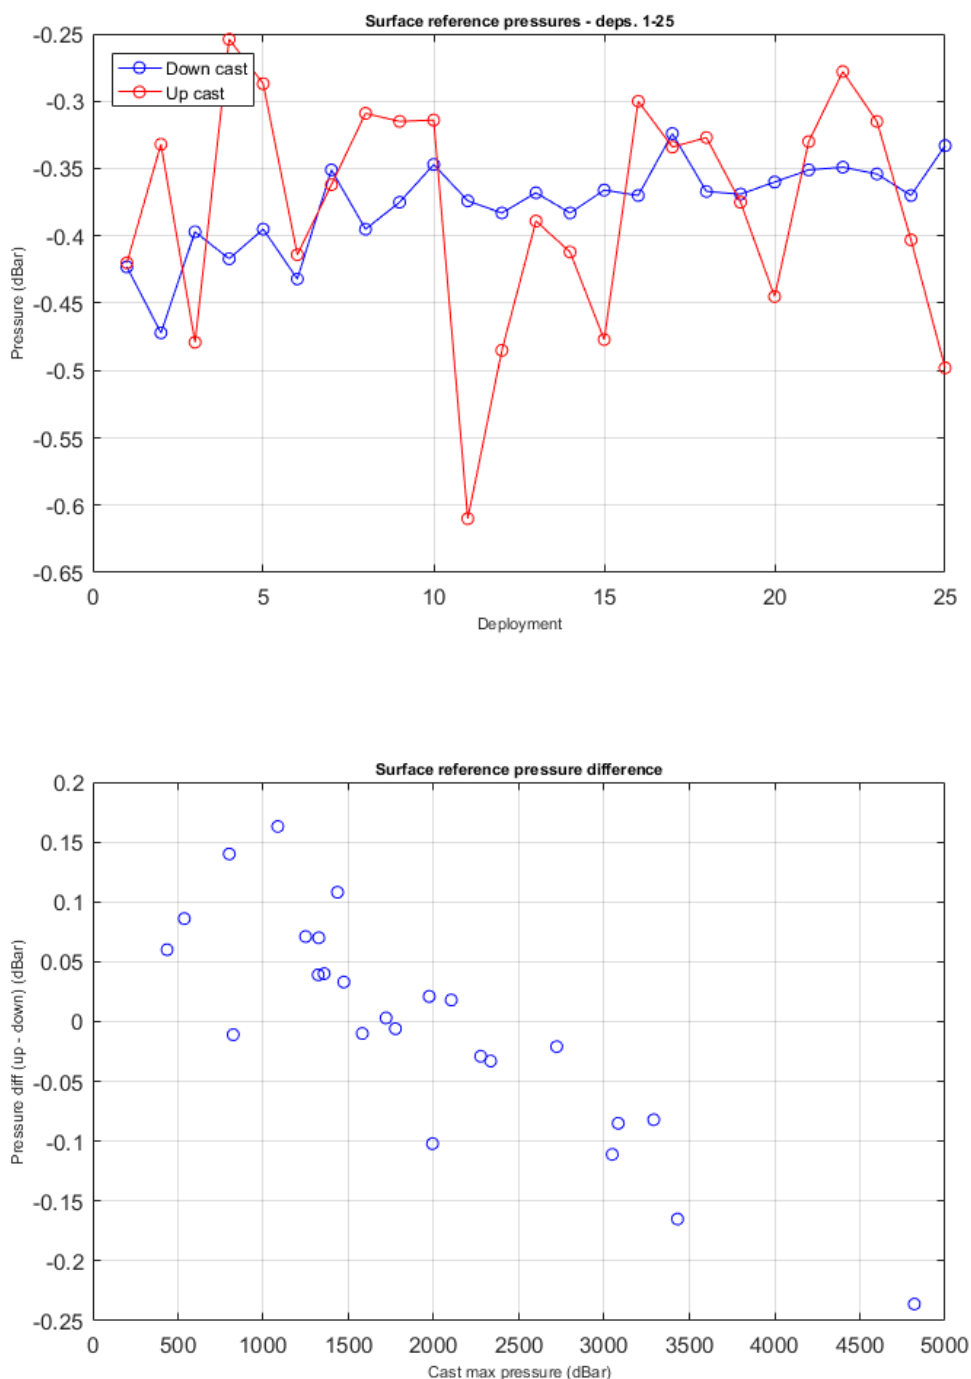


Figure 2 CTD pressure offsets

The difference between the primary and secondary temperature sensors on the downcast is plotted below. Most deployments plot within $\pm 0.001^{\circ}\text{C}$ of zero – outliers result from sampling in regions of high vertical temperature gradient as supported by the similarity between the temperature and conductivity difference shown in Figure 3. This indicates neither sensor has drifted significantly from its calibration.

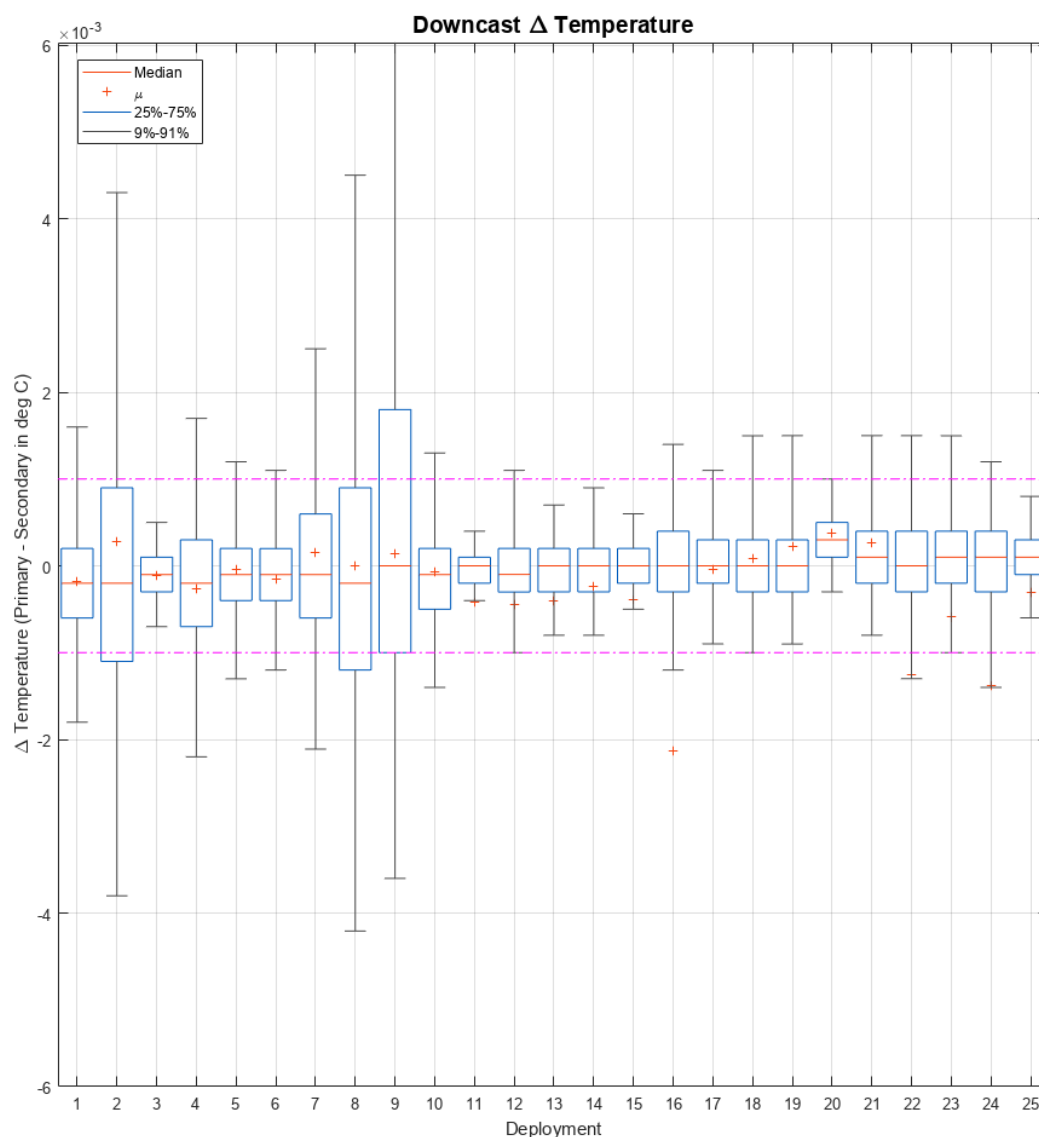


Figure 3 Difference between primary and secondary temperature sensors

3.3 Conductivity Calibration

Discrepancies and possible sampling problems between bottle and CTD salinities for the primary conductivity sensor would show in Figure 4; the plot of calibrated (CTD - Bottle) salinity below. The calibration was based upon the sample data (primary/secondary) for 181/180 of the total of 270 samples taken during deployments which are below our target of 70%.

The outliers marked in Figure 4 below with magenta dots are excluded from the calibration, the outliers marked with blue dots are used in the calibration but are weighted based on their distance from the mean. Any outliers marked with red crosses or dots are also excluded from the calibration.

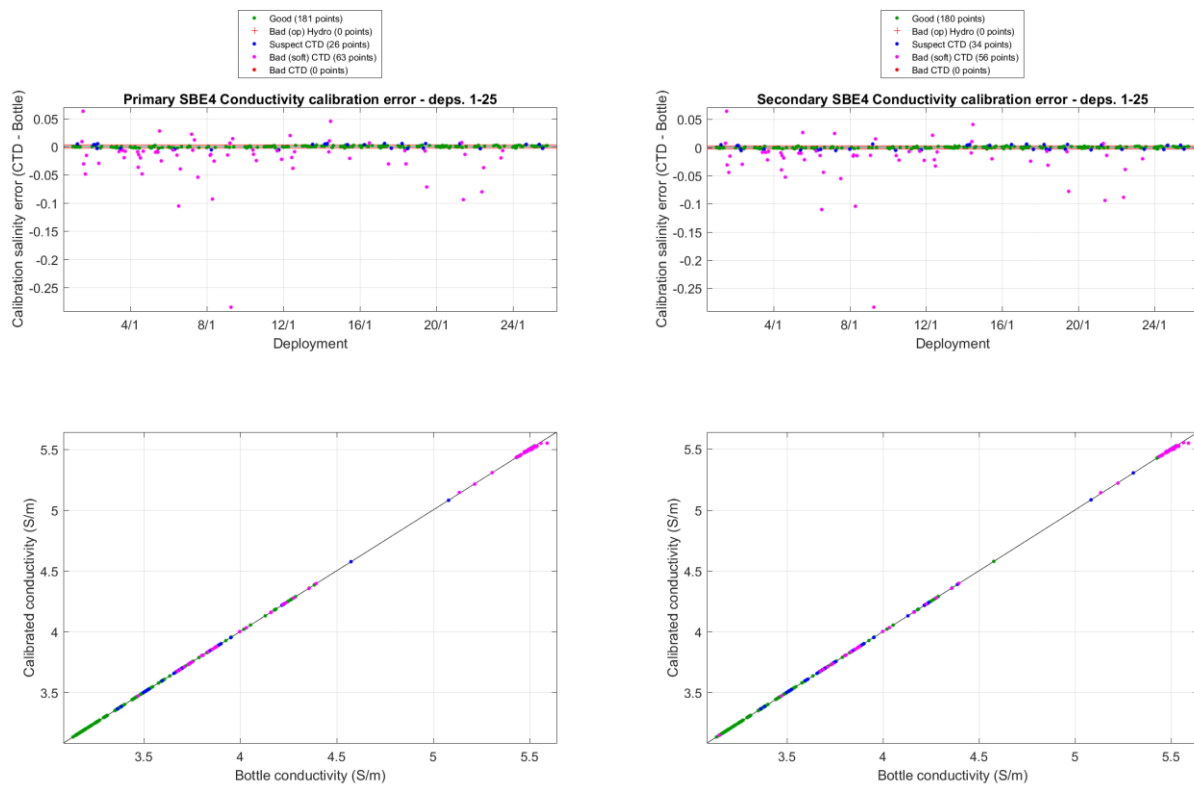


Figure 4 CTD - bottle salinity plot

The box plot of calibrated downcast conductivities (primary - secondary) for all deployments in Figure 5 shows that the calibrated conductivity cell responses corresponded very well.

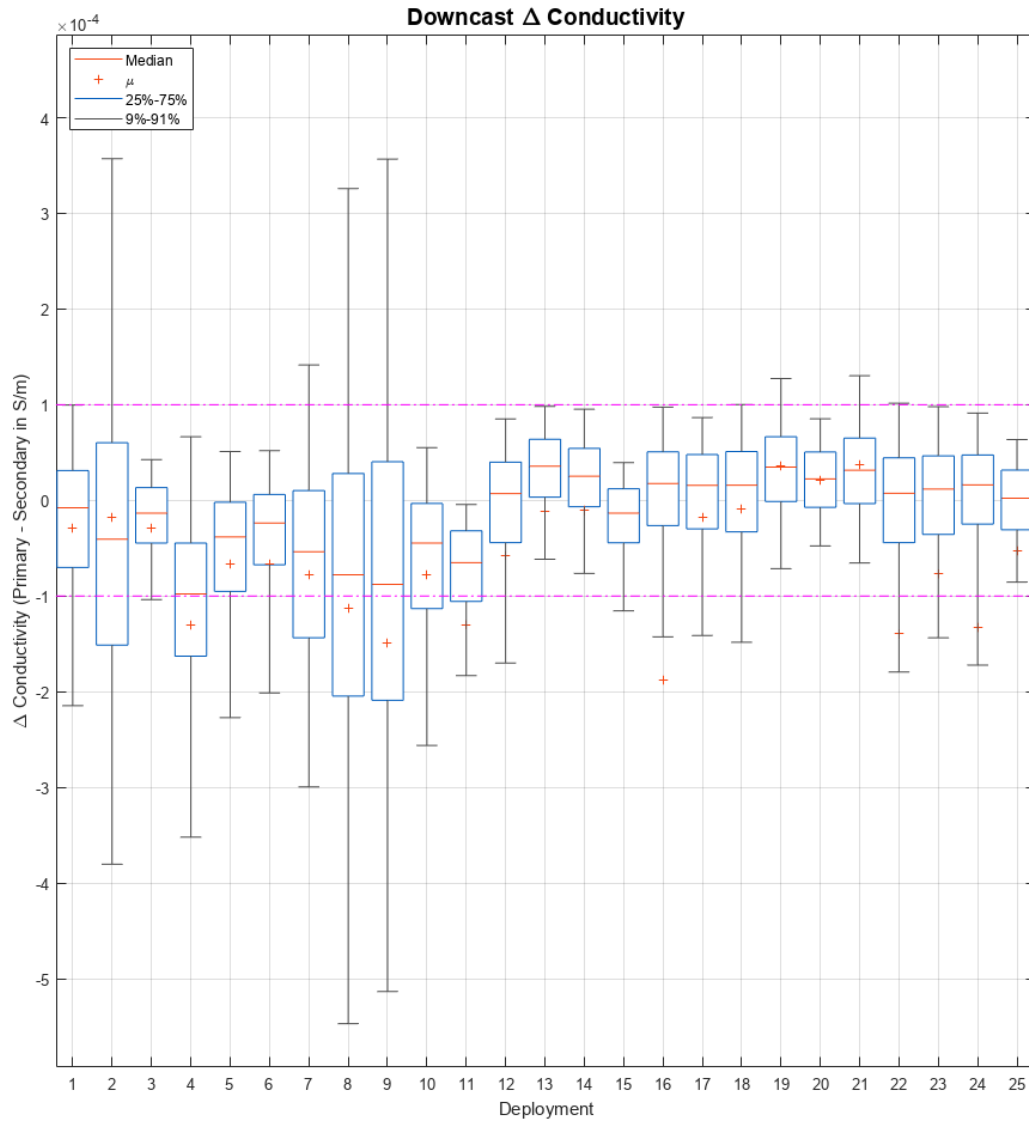


Figure 5 Difference between primary and secondary conductivity sensors

The final result for the primary and secondary conductivity sensors with respect to their original calibrations are shown in Table 2 and Table 3.

Sensor Group	Deployments	Scale Factor		Offset		Salinity (PSU)	
		a1	±	a0	±	Residual SD	M.A.D.
Primary	1-25	0.99965	0.00040217	0.0006482	0.0018269	0.0013062	0.0012365
Secondary	1-25	0.99975	0.00041159	-0.00011486	0.0018925	0.0013749	0.0011726

Table 2 Conductivity calibration with respect to manufacturers' calibration coefficients and post-calibration results

Conductivity Sensor	Deployments	CPcor	±
Primary	1-25	-9.0759e-08	1.1921e-07
Secondary	1-25	-1.0088e-07	1.2901e-07

Table 3 Calculated CPcor for primary and secondary compared to the manufacturer nominal value of -9.5700e-08

This is a good calibration. We normally aim for a S.D. of 0.002 PSU for 'typical' oceanographic voyages. The above calibration factors were applied to all deployments. Full plots of residuals before and after calibration are available in Conductivity Calibration Residual Plots.

Data from the primary conductivity and temperature sensors were used to produce the averaged salinities with secondary sensors included with a suffix '_2'.

3.4 Dissolved Oxygen Sensor Calibration

3.4.1 SBE calibration procedure

AN64: *SBE 43 Dissolved Oxygen Sensor - Background Information, Deployment Recommendations, and Cleaning and Storage* (Sea-Bird, 2013) describes the SBE43 as “a polarographic membrane oxygen sensor having a single output signal of 0 to +5 volts, which is proportional to the temperature-compensated current flow occurring when oxygen is reacted inside the membrane. A Sea-Bird CTD that is equipped with an SBE43 oxygen sensor records this voltage for later conversion to oxygen concentration, using a modified version of the algorithm by Owens and Millard (1985)”.

Calibration involves performing a linear regression, as per *AN64-2: SBE 43 Dissolved Oxygen Sensor Calibration and Data Corrections* (Sea-Bird, 2012) to produce new estimates of the calibration coefficients *Soc* and *Voffset*. These new coefficients are used, along with the other, manufacturer-supplied coefficients, to derive oxygen concentrations from the sensor voltages.

3.4.2 Results

Deeper casts (>1000m) are known to be affected by pressure-induced hysteresis with this sensor. This is corrected automatically within CapPro using the method discussed in *AN64-3: SBE 43 Dissolved Oxygen (DO) Sensor - Hysteresis Corrections* (Sea-Bird, 2014).

There is a small mismatch between downcast and upcast dissolved oxygen due to the response time of the sensor. No correction for the sensor lag effect has been applied.

A single calibration group was used with the associated SBE43 up-cast data to compute the new *Soc* and *Voffset* coefficients. The plot below is of CTD - bottle oxygen differences for both upcast and downcast data (red indicates ‘bad’ data; + for upcast and square for downcast).

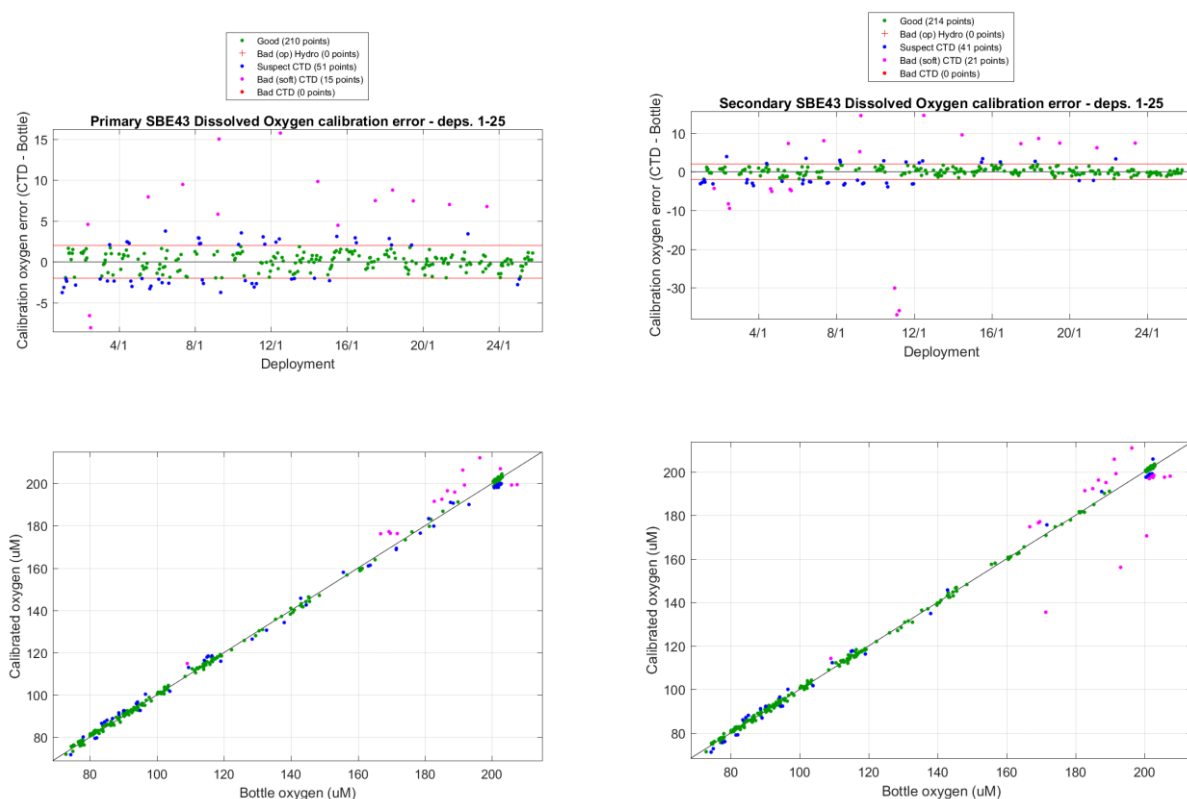


Figure 6 Dissolved Oxygen Difference with upcast CTD data (SBE43 - Bottle)

The box plot of calibrated downcast Dissolved Oxygen readings (primary - secondary) for all deployments in Figure 7 shows that the calibrated Dissolved Oxygen sensor responses corresponded well.

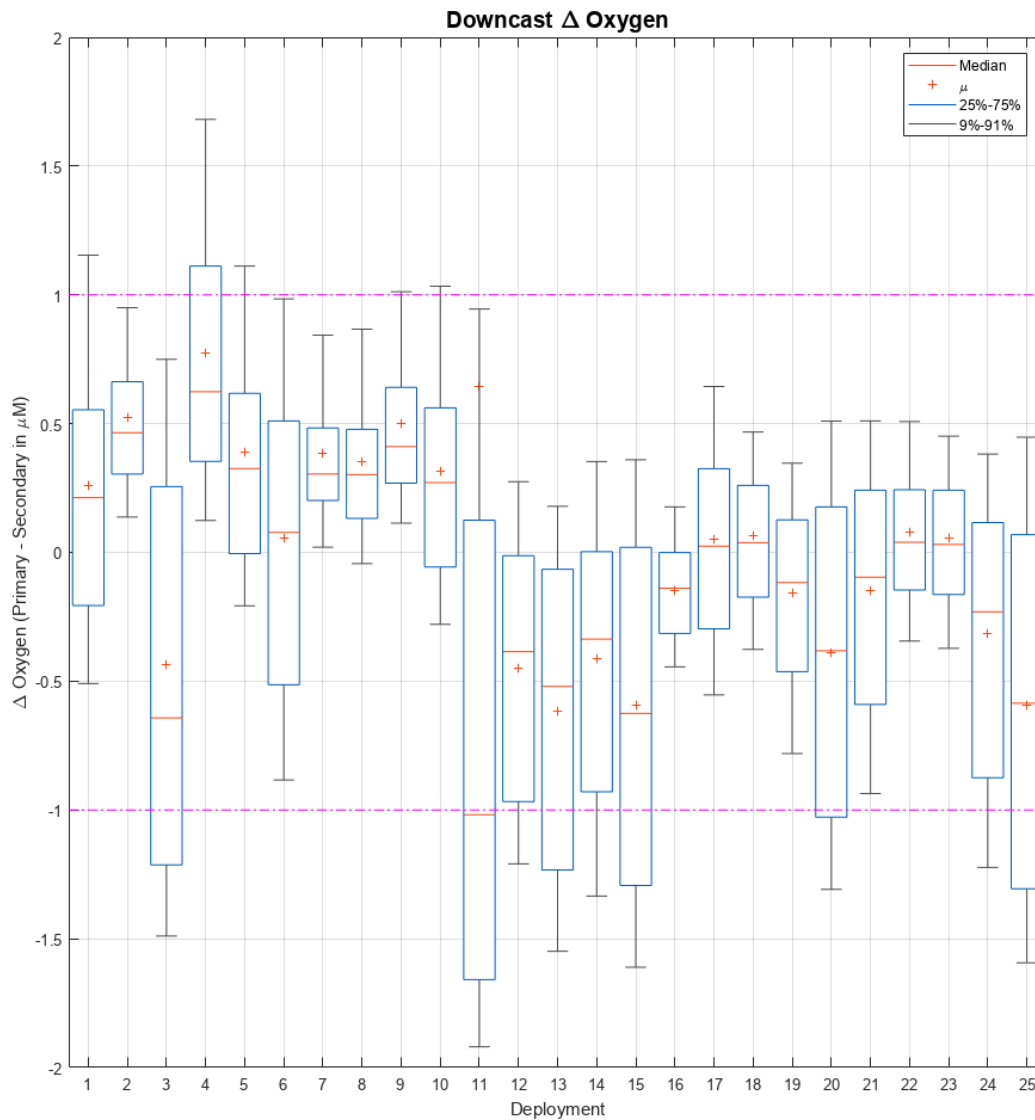


Figure 7 Difference between primary and secondary Dissolved Oxygen sensors

The old and new *Soc* and *Voffset* values for DO sensors are listed in Table 4 below. The *Soc* value is a linear slope scaling coefficient; *Voffset* is the fixed sensor voltage at zero oxygen. As expected, over time, the increasing *Soc* scale factors show the SBE43 sensor is losing sensitivity. Full plots of residuals before and after calibration are available in Dissolved Oxygen Calibration Residual Plots.

The calibrations were applied for each sensor and the averaged files were created using the result from the primary sensor.

Sensor	Calibration Source	Deployments	Calibration Coefficients				Dissolved Oxygen (μM)	
			<i>Voffset</i>	\pm	<i>Soc</i>	\pm	Residual SD	M.A.D.
Primary DO	CapPro	1-25	-0.48907	0.0017408	0.53547	0.0012294	0.89089	1.003
	CSIRO Cal Lab	1-25	-0.5054		0.52968			
Secondary DO	CapPro	1-25	-0.4604	0.0017259	0.49629	0.0010463	0.92741	0.74045
	Sea-Bird	1-25	-0.475		0.478			

Table 4 Dissolved oxygen calibrations

3.5 Other sensors

The C-Star transmissometer was used on all deployments. It was calibrated by the manufacturer with meter outputs with the beam blocked, in air with a clear beam path and with clean water in the path. These values are used to determine a scale and offset for use in SBE Data Processing software to convert the raw counts to a beam transmittance output of 0-100 percent.

The WET labs ECO Fluorometer-Scattering sensor was used for all deployments. The fluorometer has been calibrated with manufacturer supplied coefficients to give outputs in mg/m^3 . The scattering (OBS) has been calibrated with manufacturer supplied coefficients to give outputs in m^{-1}/sr . The WET labs ECO CDOM sensor was also used for all deployments. The CDOM ECO measures Colored Dissolved Organic Matter fluorescence and has been calibrated with manufacturer supplied coefficients to give outputs in ppb.

The Seapoint Nephelometer was used for all deployments. The Seapoint Turbidity Meter detects light scattered by particles suspended in water from a small volume within 5 centimeters of the sensor. It generates an output voltage proportional to turbidity or suspended solids. The output of the sensor is within the range 0-5000, however, for this voyage it recorded only values of 0-1 indicating that it may be out of calibration or need a repair.

3.6 Bad data detection

The limits for each sensor are configured in CNV_to_Scan conversion software and are written to the NetCDF scan file. Typical limits used for the sensor range and maximum second difference are in Table 5 below. The rejection rate is recorded in the CapPro processing log file.

Sensor	Range minimum	Range maximum	Maximum Second Difference
Pressure	-7	6500	0.5
Temperature	-2	40	0.05
Conductivity	-0.01	7	0.01
Oxygen	-1	500	0.5
Fluorometer	0	100	0.5
PAR	-5	2000	0.5
Transmissometer	0	100	0.5
Turbidity, Seapoint	-5	5000	10
Transmissometer	0	100	0.5
CDOM, Wetlabs	-5	515	0.5
Turbidity, Wetlabs	0	3	1e-4

Table 5 Sensor limits for bad data detection

3.7 Heave Filtering

Sensor data impacted by ship heave impeding the CTD deployment is filtered out in three stages, and applied during data binning. The first stage detects negative acceleration of the CTD which can cause trailing mixed water to be pumped through the sensors. The second stage looks at all negative density gradients and flags readings which are above 10 times the standard deviation of all negative gradients, for 2 seconds. The third stage flags any pressure reversals which are greater than the height of the CTD sensor pump inlet above the frame.

3.8 Averaging

The calibrated data were ‘filtered’ to remove pressure reversals and binned into the standard product of 1 decibar averaged NetCDF files. The binned values were calculated by applying a linear, least-squares fit as a function of pressure to the sensor data for each bin, using this to interpolate the value for the bin mid-point. This method is used to avoid possible biases which would result from averaging with respect to time.









Each binned parameter is assigned a QC flag. Our quality control flagging scheme is described in *Data Quality Control Flags* (Pender, 2000).

The QC Flag for each bin is estimated from the values for the bin components. The QC Flag for derived quantities, such as Salinity and Dissolved Oxygen are taken to be the worst of the estimates for the parameters from which they are derived.

4 References

- Tim O'Hara. (2021). *The RV Investigator. Voyage Plan in2021_v04*. Retrieved from Marine National Facility: Voyage Plans and summaries: <https://mnf.csiro.au/en/Voyages/Voyage-Catalogue>
- Pender, L. (2000). *Data Quality Control Flags*. Retrieved from Oceans & Atmosphere Information and Data Centre: http://www.cmar.csiro.au/datacentre/ext_docs/DataQualityControlFlags.pdf
- Sea-Bird. (2012). *AN64-2: SBE 43 Dissolved Oxygen Sensor Calibration and Data Corrections*. Retrieved from Sea-Bird Electronics: <https://www.seabird.com/asset-get.download.jsa?code=251034>
- Sea-Bird. (2013). *AN64: SBE 43 Dissolved Oxygen Sensor - Background Information, Deployment Recommendations, and Cleaning and Storage*. Retrieved from Sea-Bird Electronics: <https://www.seabird.com/asset-get.download.jsa?code=251036>
- Sea-Bird. (2014). *AN64-3: SBE 43 Dissolved Oxygen (DO) Sensor - Hysteresis Corrections*. Retrieved from Sea-Bird Electronics: <https://www.seabird.com/asset-get.download.jsa?code=251035>

Appendix I: Conductivity Calibration Residual Plots

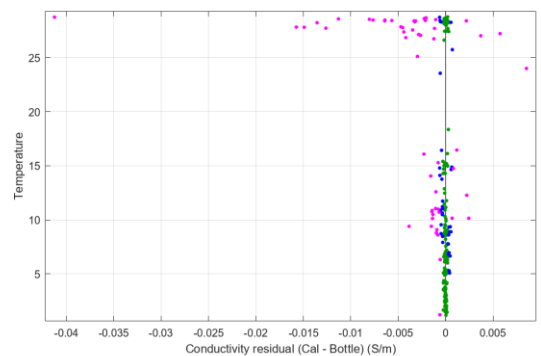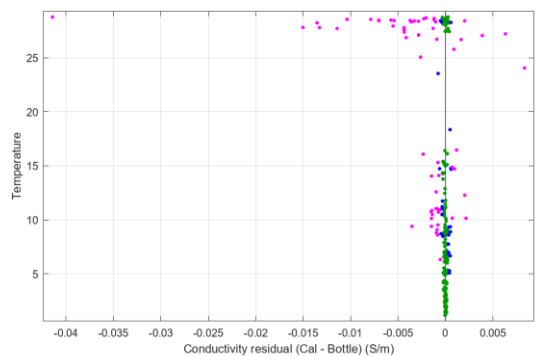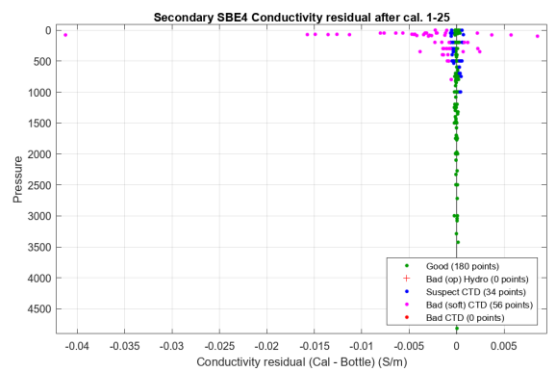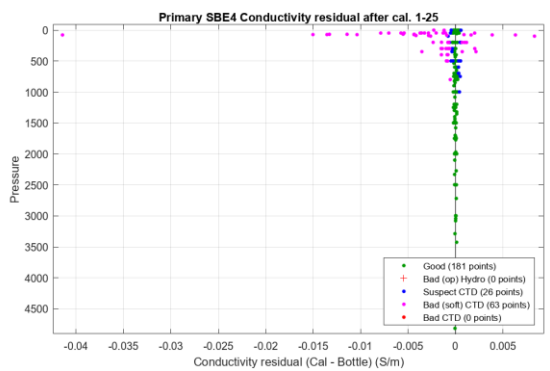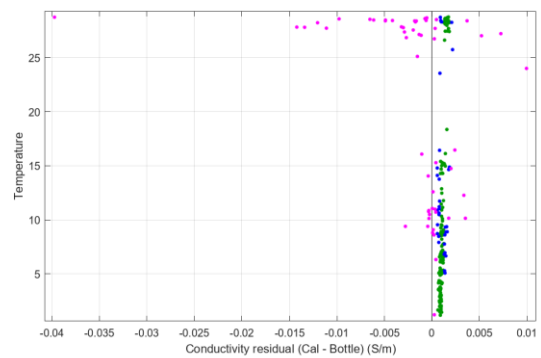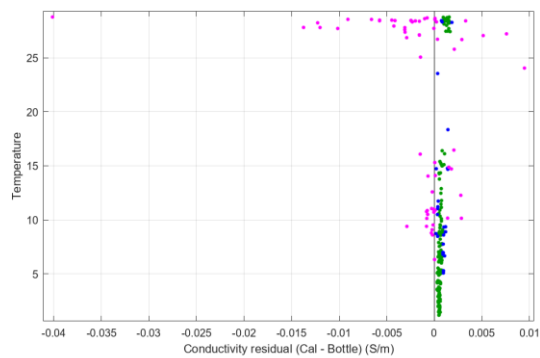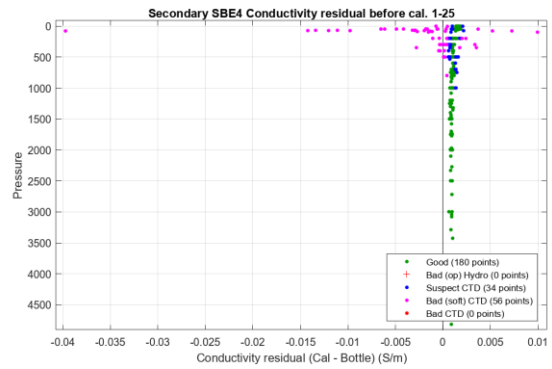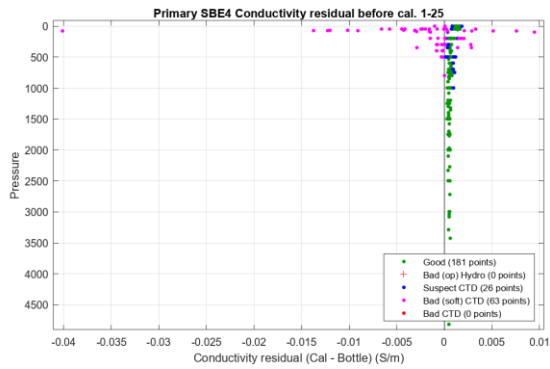

Appendix II: Dissolved Oxygen Calibration Residual Plots

